


Davide Ferri :: Paul Scherrer Institut

# **Infrared spectroscopy**


Molecular aspects of catalysts and surfaces :: ETHZ

# The electromagnetic spectrum

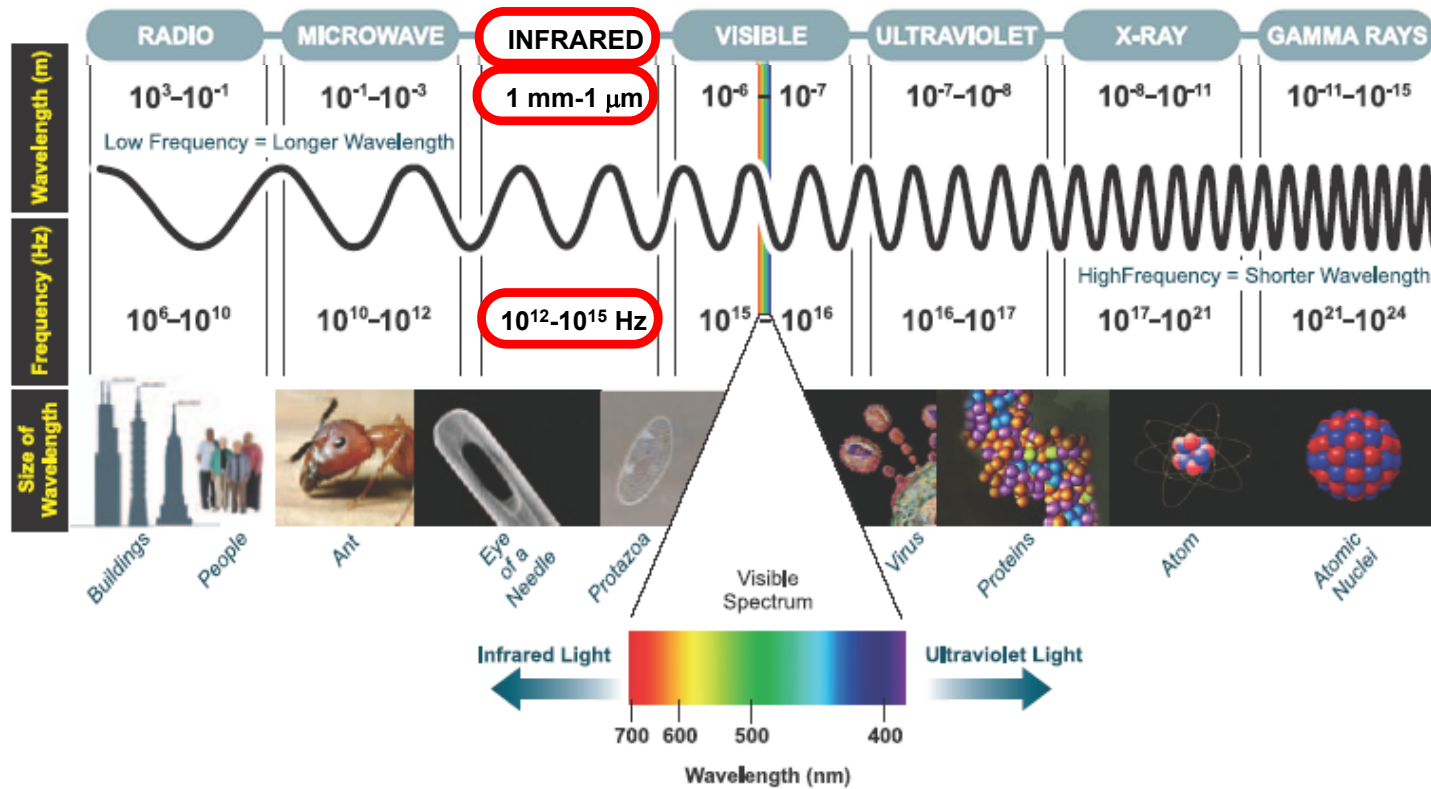

source: Andor.com

# Importance of IR spectroscopy in catalysis

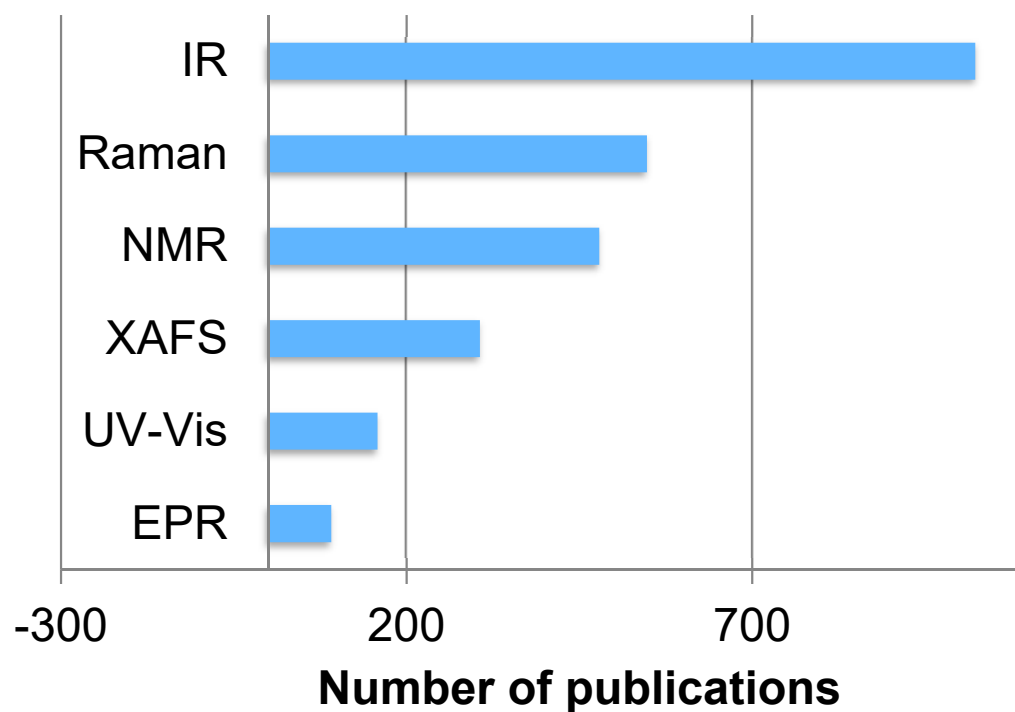


- pros
  - economic
  - non-invasive
  - versatile (e.g. solid, liquid, gas, interfaces)
  - very sensitive (concentration)
  - fast acquisition (down to ns!)
- cons
  - no atomic resolution

Number of publications containing *in situ*, *catalysis*, and respective method

Source: ISI Web of Knowledge (Sept. 2008)

# Infrared spectroscopy

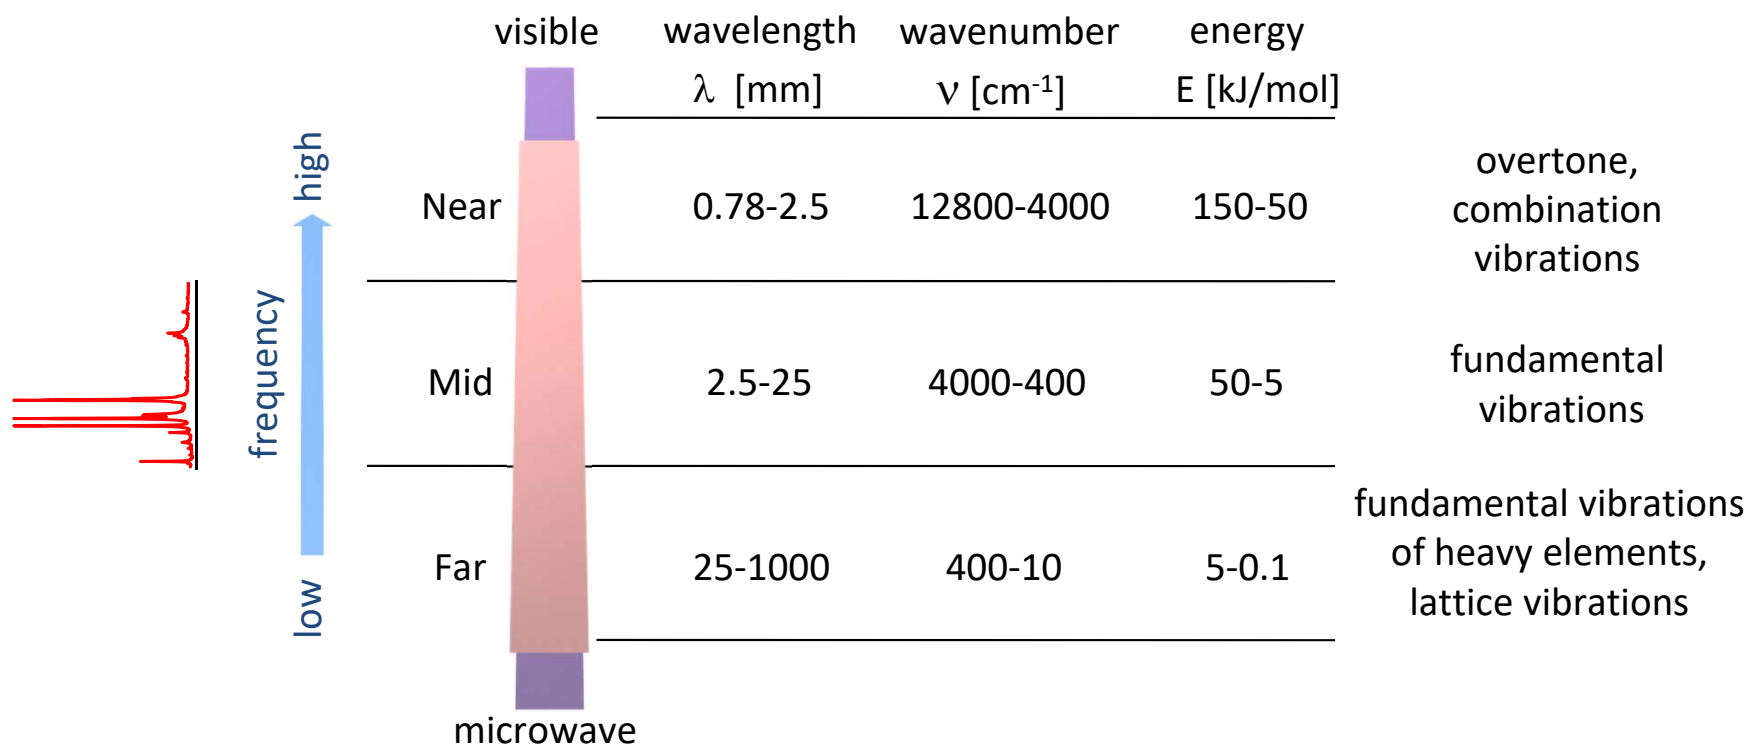


## Why IR spectroscopy


- ‘quality control’: identification of compounds according to their fingerprint spectrum
  - also inorganic materials, e.g. metal oxides
  - ex situ, but also after degassing in cell (vacuum)
- Identification of surface sites | Detailed characterization of surface
  - use of molecular probes
  - in situ experiments, controlled dosage of probe
- Identification of surface sites under reaction conditions
  - in situ/operando experiments to obtain molecular reaction mechanism, exposure to reaction conditions

# Vibrational spectroscopy


- Interaction with matter
  - energy causes vibration of molecular bonds
  - energy is absorbed in correspondence of vibrational modes
  - an absorption band is generated

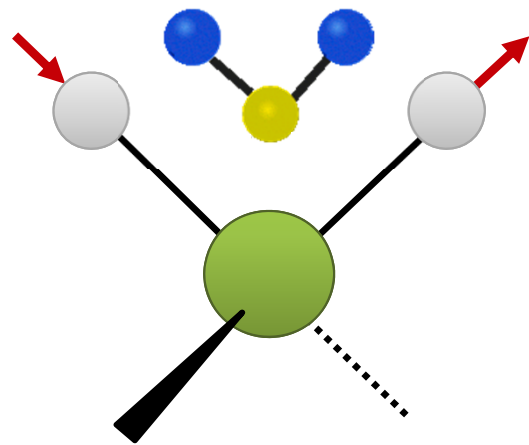

asymmetric stretching

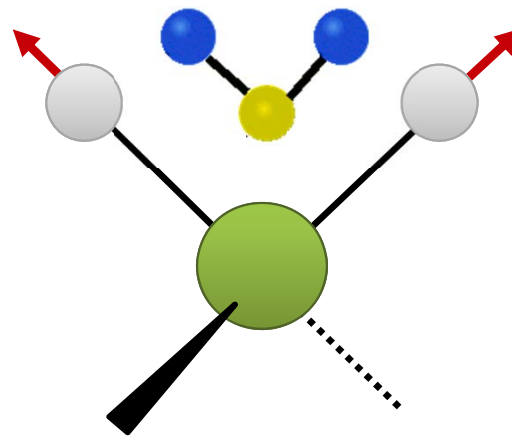


symmetric stretching

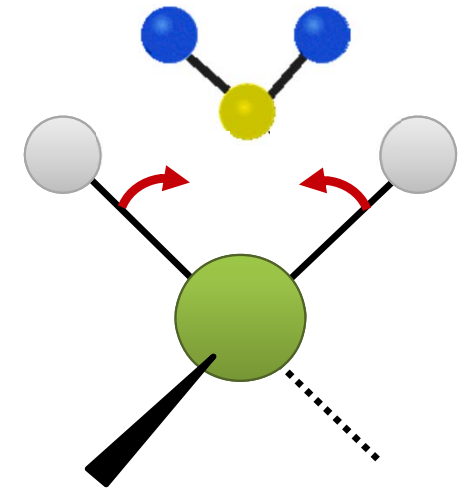

bending

← energy

# Vibrations

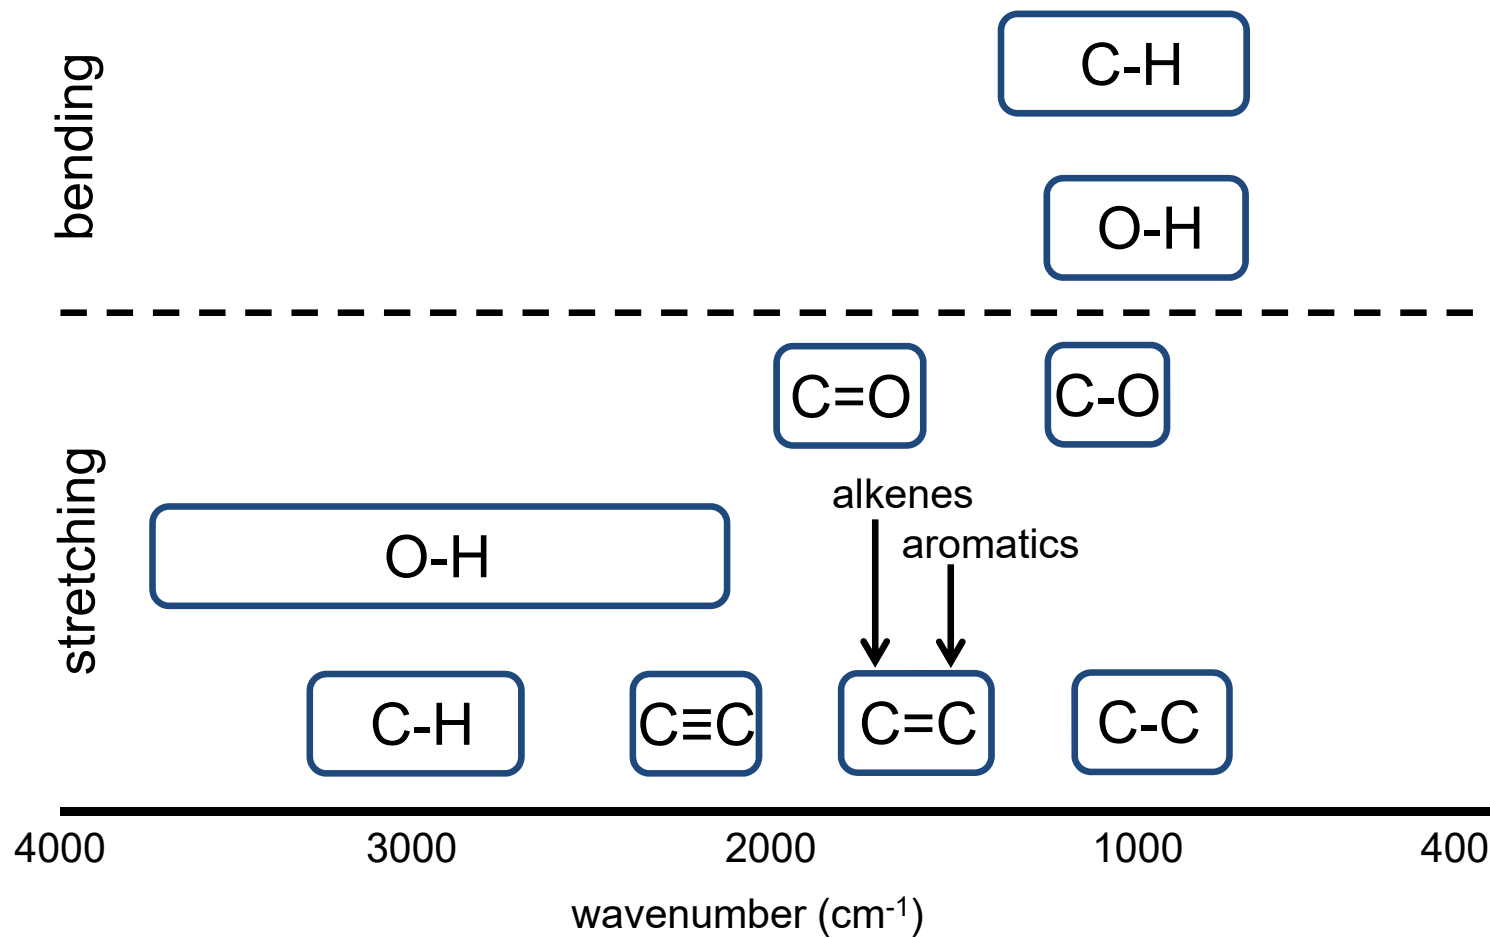


# Vibrations

- Why do vibrations appear in the IR spectrum?


selection rule

$$\left( \frac{\partial \mu}{\partial Q} \right) \neq 0$$




molecular dipole moment  $\mu$  must change due to vibration or rotation along its coordinate (so called, normal mode or normal coordinate,  $Q$ )






N=3, non-linear, 3 fundamental modes

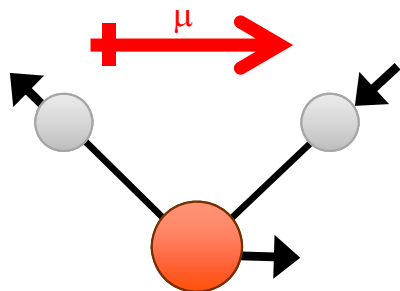


**3756 cm<sup>-1</sup>**

asymmetric stretching

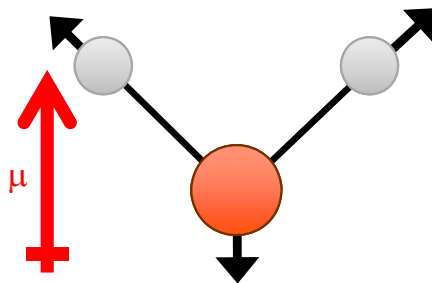

**3657 cm<sup>-1</sup>**

symmetric stretching

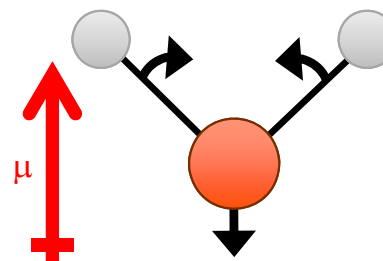


**1595 cm<sup>-1</sup>**

scissoring (bending)


**All modes IR active**

# Gas and liquid phase H<sub>2</sub>O

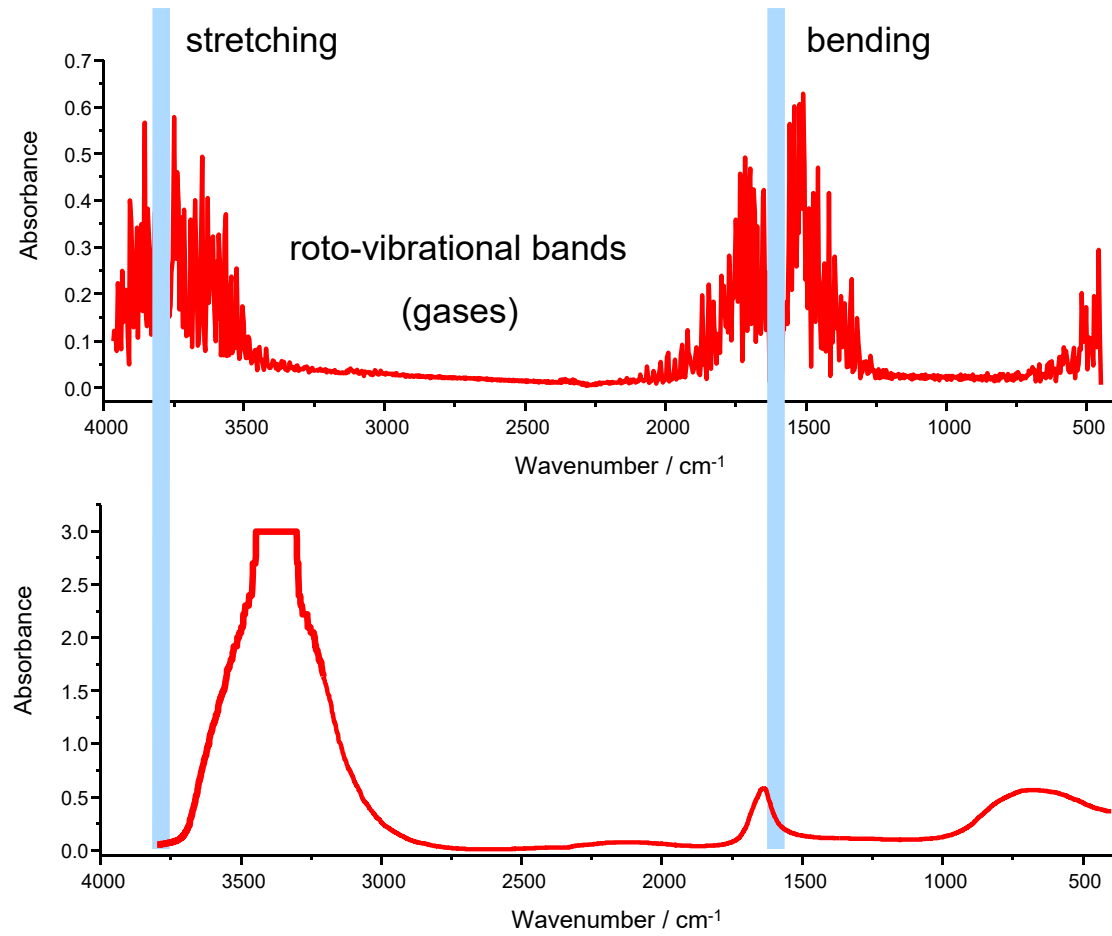

# Vibrations

- Harmonic oscillator
  - The stretching frequency of a bond can be approximated by Hooke's law. Two atoms and the connecting bond are treated as a harmonic oscillator composed of two masses (atoms) joined by a spring.

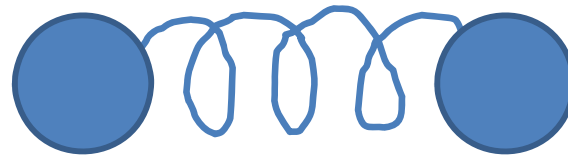

$$\nu = \frac{1}{2\pi} \sqrt{\frac{k}{\mu}}$$

k: force constant

$$\mu = \frac{m_1 \times m_2}{m_1 + m_2}$$

m: reduced mass

# Vibrations

$$\nu = \frac{1}{2\pi} \sqrt{\frac{k}{\mu}}$$

C-C  
1200 cm<sup>-1</sup>

C=C  
1650 cm<sup>-1</sup>

C≡C  
2200 cm<sup>-1</sup>

larger k

C-H  
3000 cm<sup>-1</sup>

C-D  
2100 cm<sup>-1</sup>


C-C  
1200 cm<sup>-1</sup>

C-O  
1100 cm<sup>-1</sup>

C-Cl  
800 cm<sup>-1</sup>

larger μ

# The spectrometer

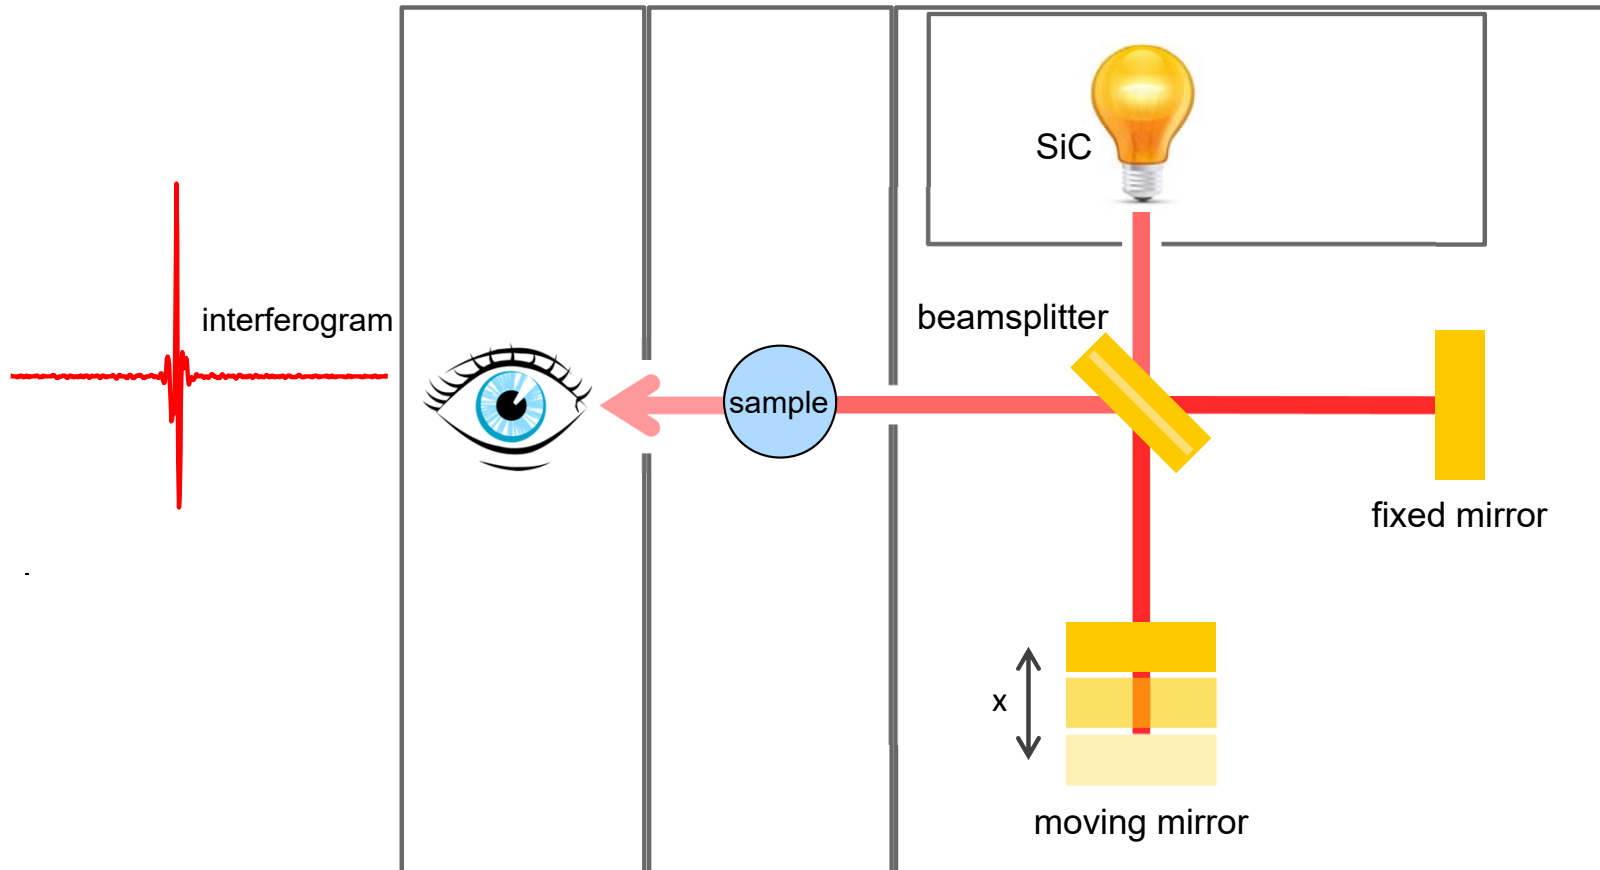

# Dispersive vs. FT

FT-IR spectrometer has significant advantages over dispersive one

- **Multiplex ( Fellgett ) advantage**

All source wavelengths are measured simultaneously


- **Throughput ( Jacquinot ) advantage**

For the same resolution, the energy throughput in an interferometer can be higher  
→ the same S/N as a dispersive-IR in a much shorter time


- **Precision ( Connes ) advantage**

The wavenumber scale of an interferometer is derived from a HeNe laser that acts as an internal reference for each scan

# The IR spectrum


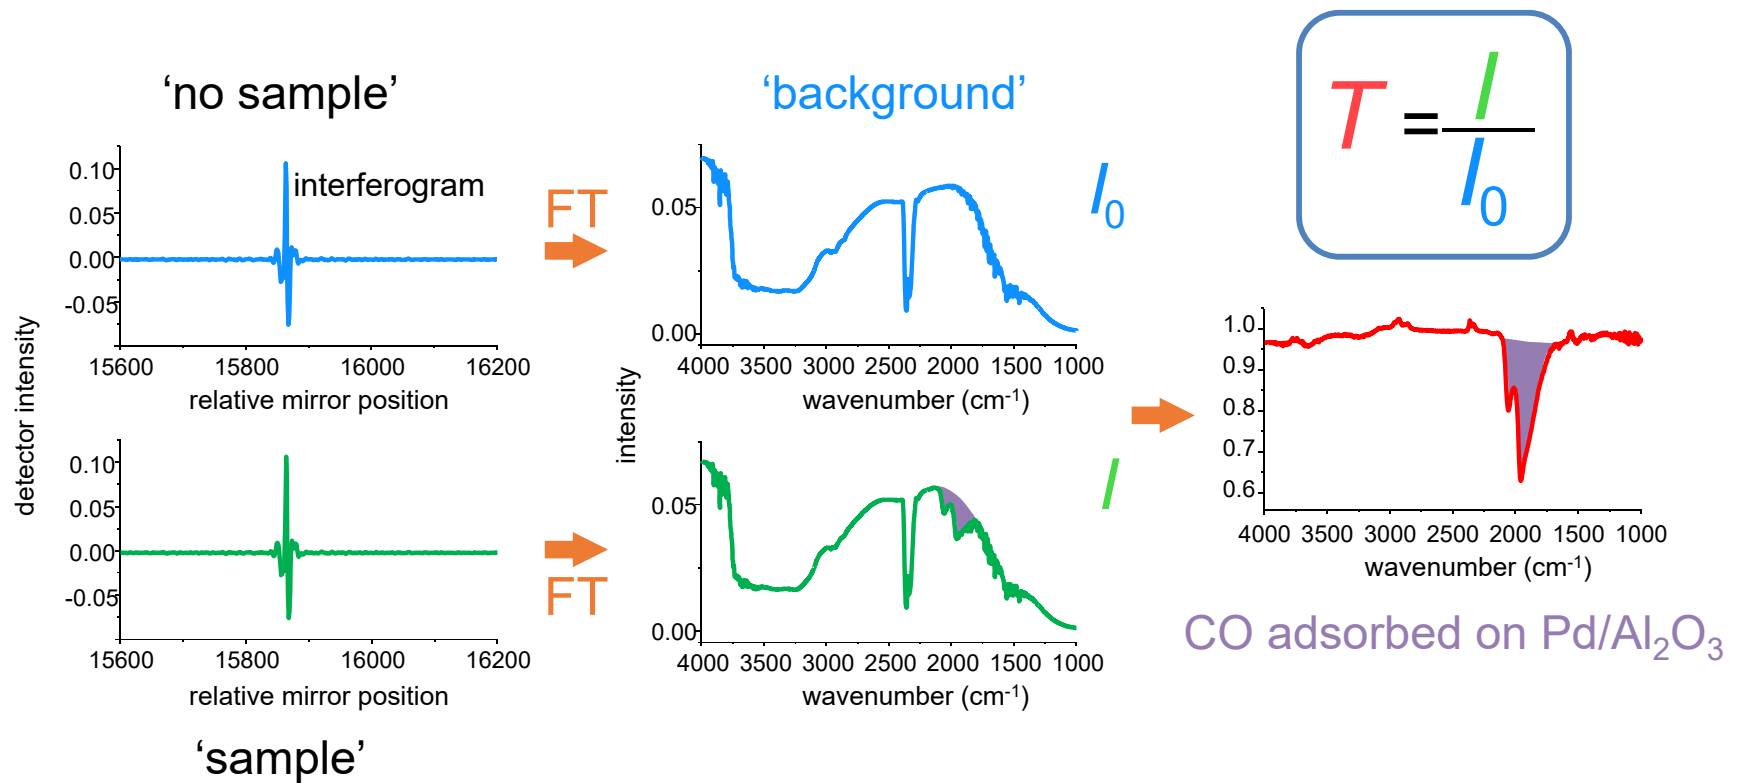


# The IR spectrum

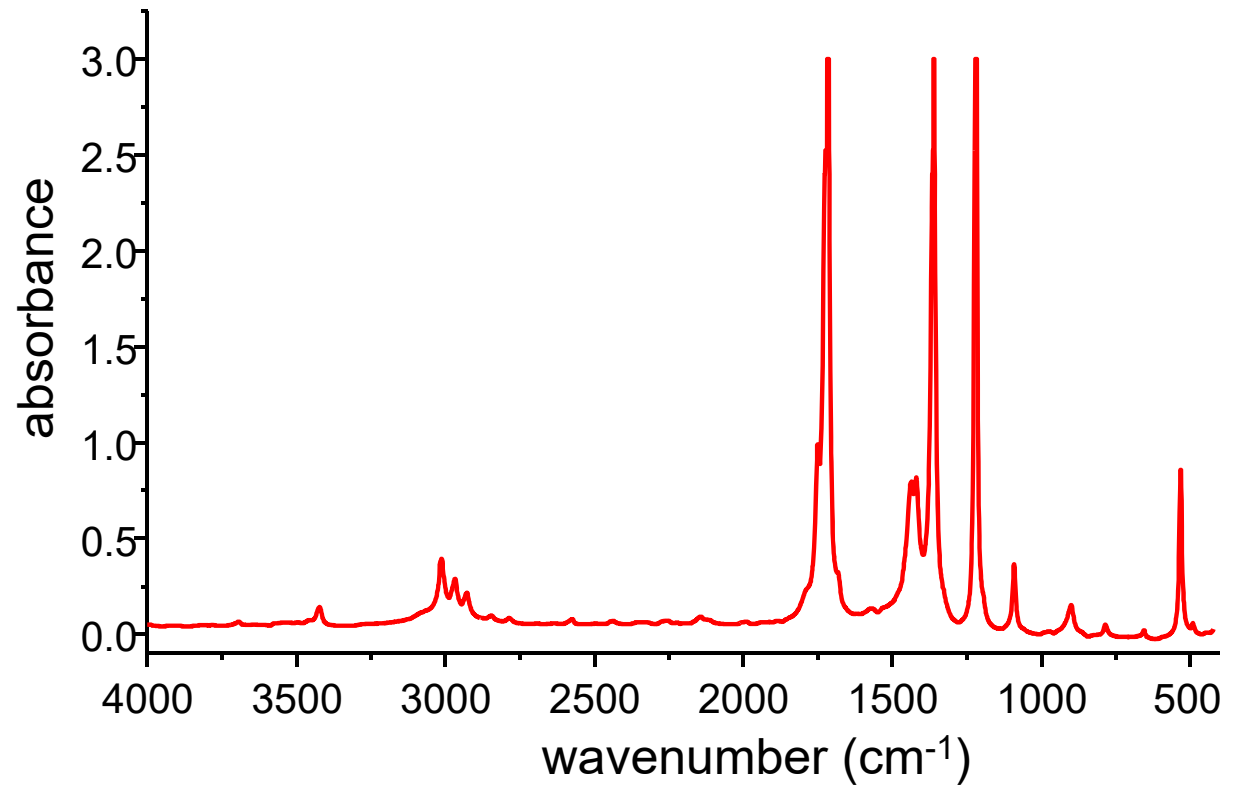




# The IR spectrum

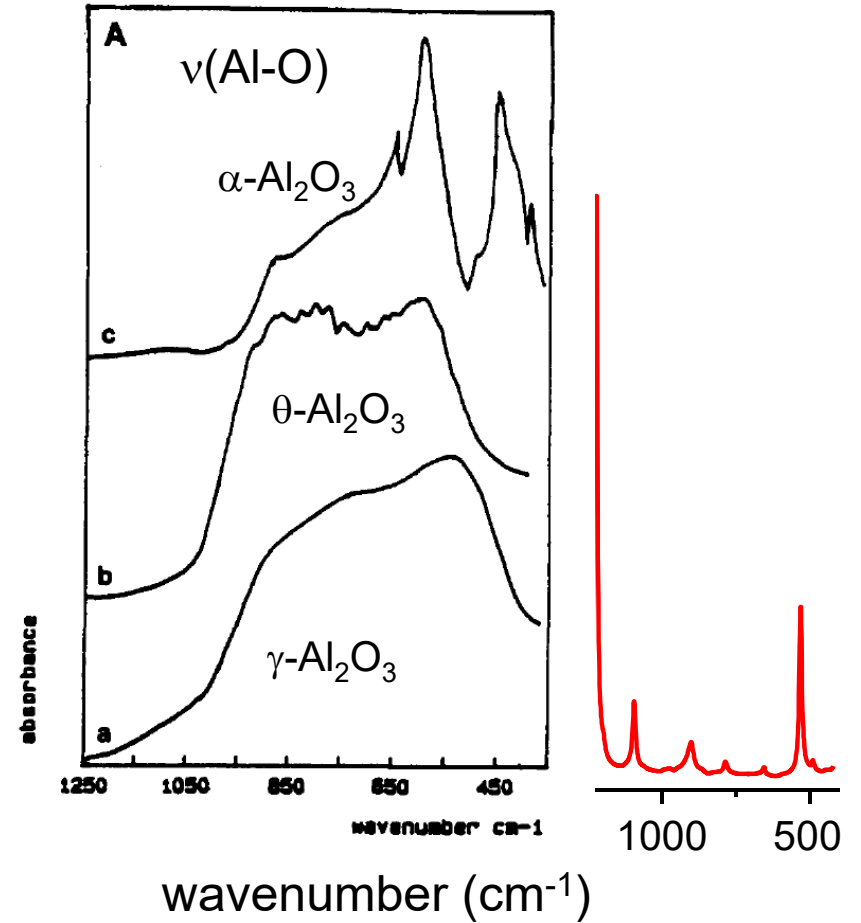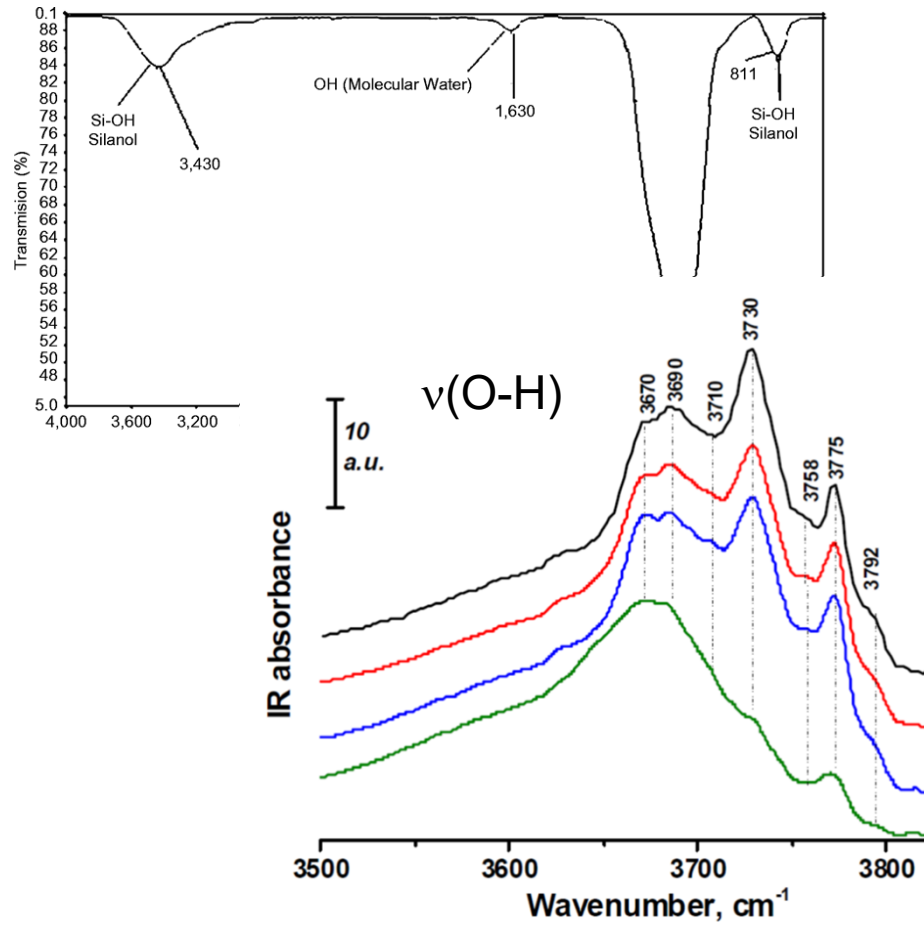


# The background

- DRIFT spectra of V-W-TiO<sub>2</sub> catalysts after adsorption of NH<sub>3</sub>
  - aspect of spectra changes with background

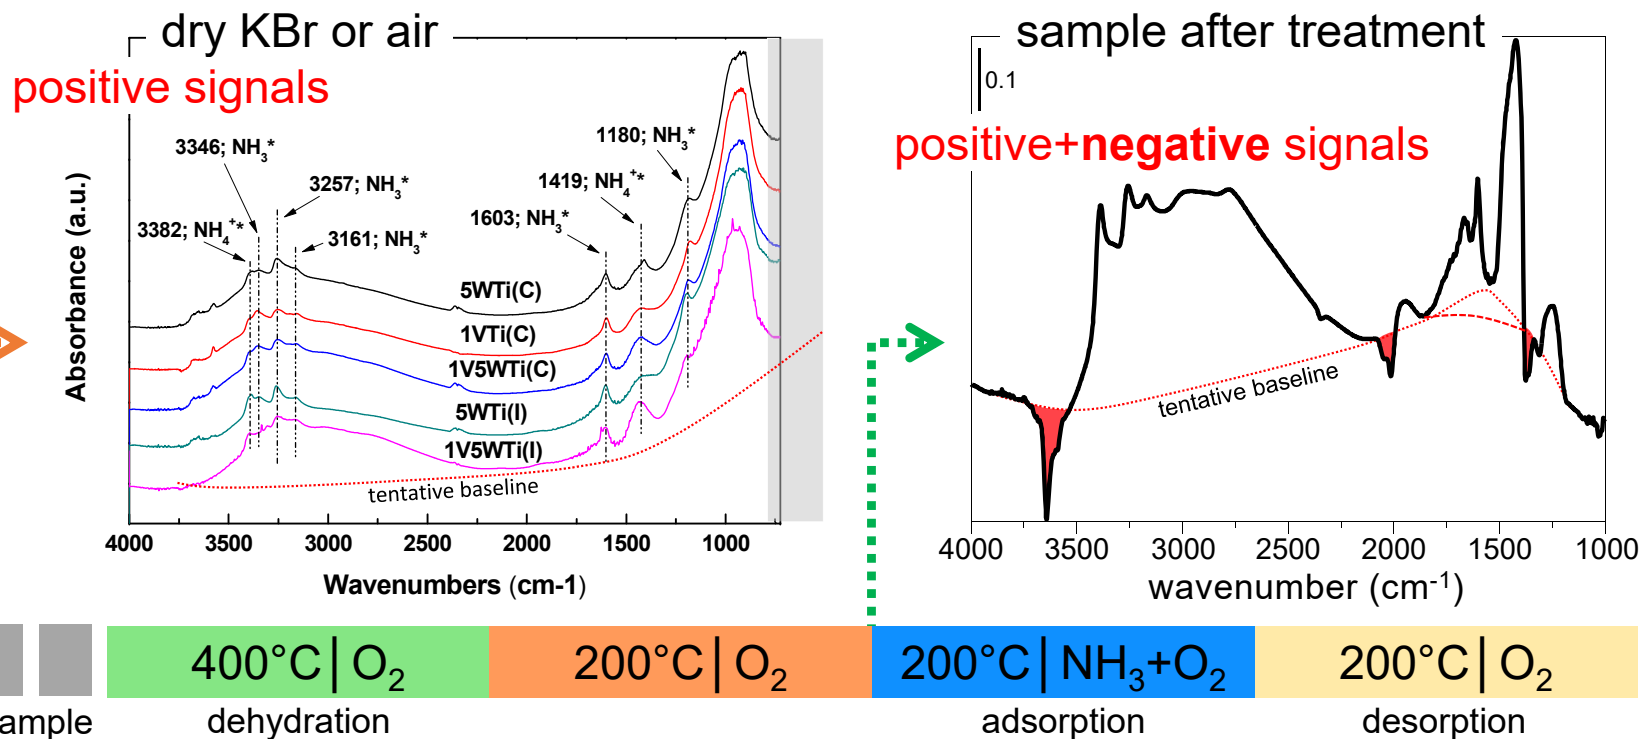


## Information on materials

- The spectrum contains information on
  - terminal O-H bonds | 3800-3600  $\text{cm}^{-1}$
  - bridge hydroxyls | Brønsted acidity
  - H-bonded hydroxyls
  - M-O and M=O bonds, bulk and surface
    - fundamental (n) and overtone ( $2 \times n$ ) modes
  - other groups, e.g. C-H, carbonates, carboxylates...

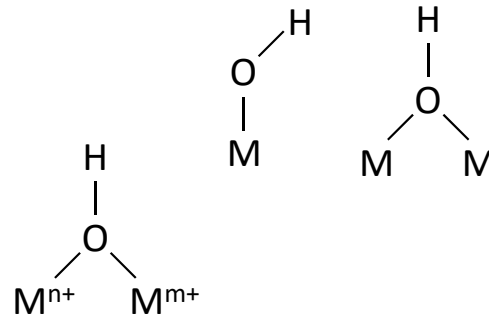

# Information on materials

- Perturbation of hydroxyls  
– adsorption of probe molecule

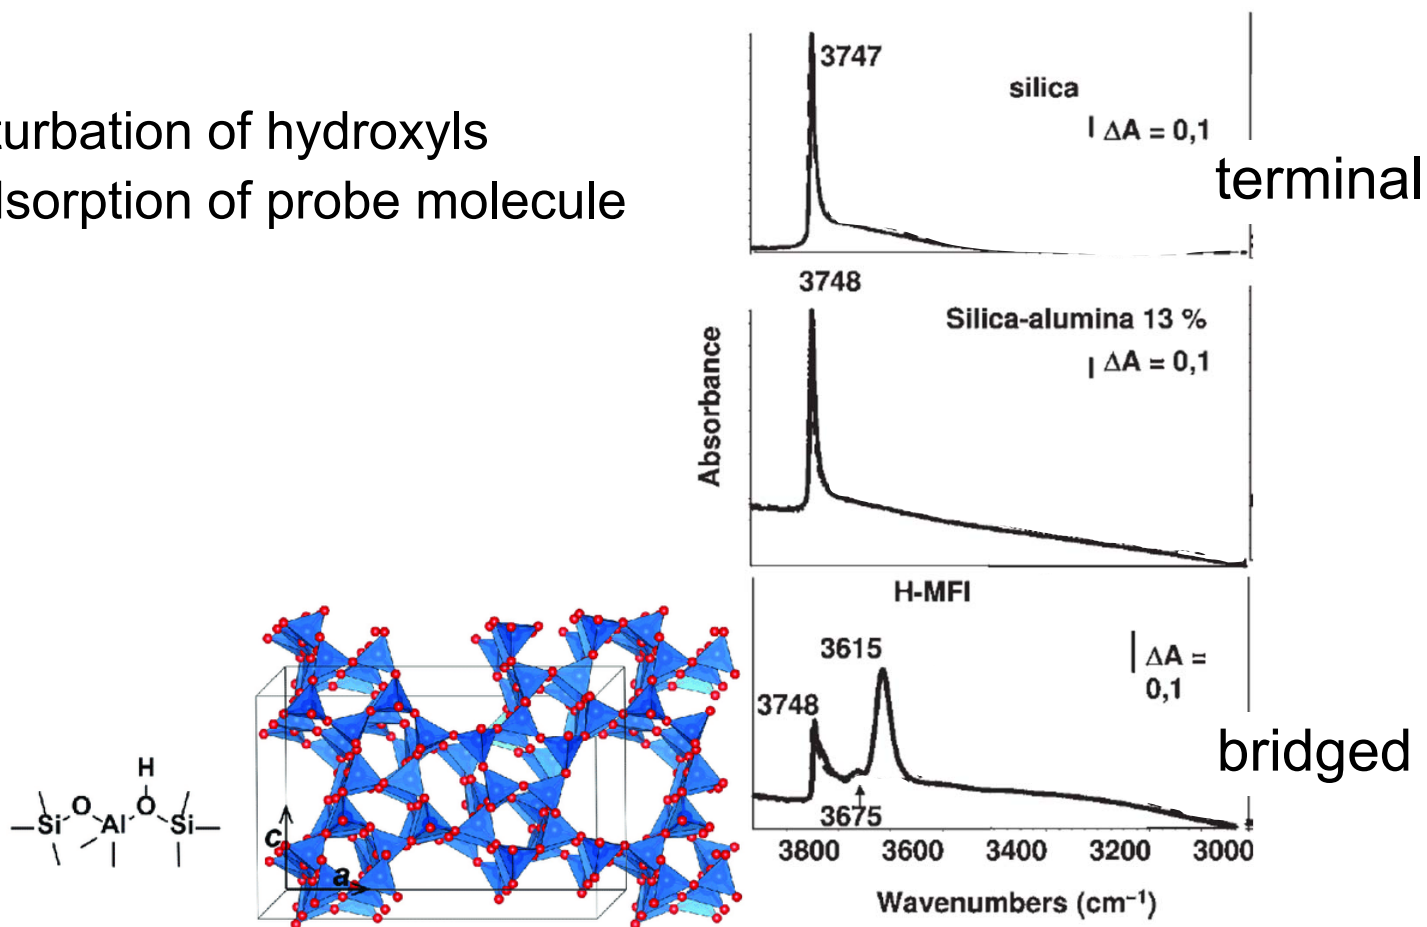


Busca, in Metal Oxide Catalysis, Wiley-VCH Verlag GmbH & Co. KGaA, Weinheim (2009) 95 | Uslamin, Zeolite-based catalysis for sustainable aromatics production, Technische Universiteit Eindhoven (2019)

## Information on materials

- Perturbation of hydroxyls
  - adsorption of probe molecule





- H-bonded hydroxyls

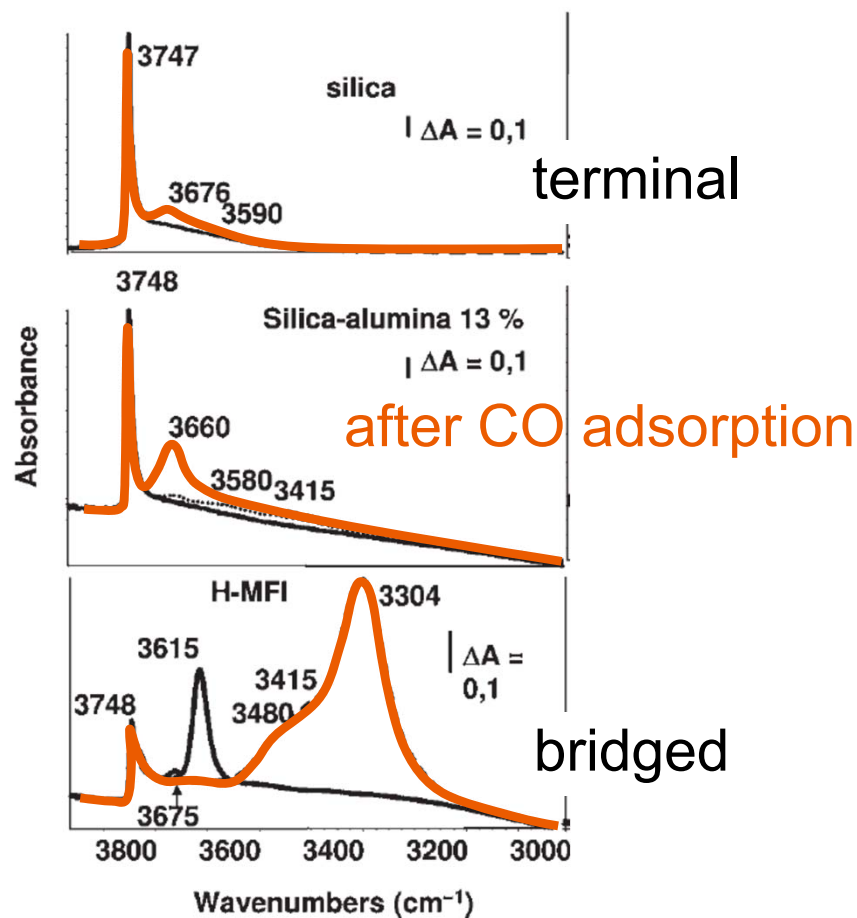

# Information on materials


- Also other disciplines...

Single model	Number of samples	Energetical value (kJ/100 g)		Proteins (g/100 g)		Fat (g/100 g)		Carbohydrates (g/100 g)		Calcium (mg/100 g)	
		Mean	± s	Mean	± s	Mean	± s	Mean	± s	Mean	± s
Calibration	19	334	154	4.1	0.7	2.7	3.0	9.4	4.2	135	22
Validation	29	268	106	3.8	0.5	1.6	1.4	8.4	4.4	125	6
Extended model	Number of samples	Energetical value (kJ/100 g)		Proteins (g/100 g)		Fat (g/100 g)		Carbohydrates (g/100 g)		Calcium (mg/100 g)	
		Mean	± s	Mean	± s	Mean	± s	Mean	± s	Mean	± s
Calibration	32	295	137	3.9	0.7	2.1	2.3	8.8	4.4	129	16
Validation	16	277	100	3.9	0.4	1.7	1.4	8.6	4.4	127	12

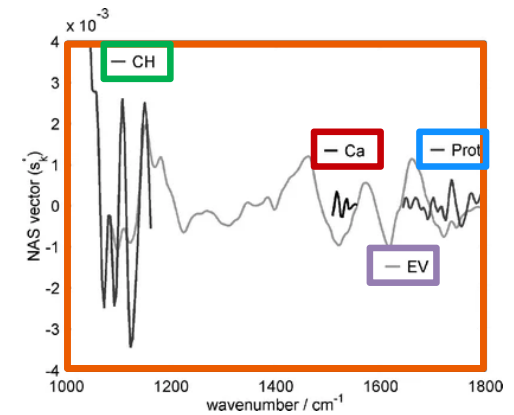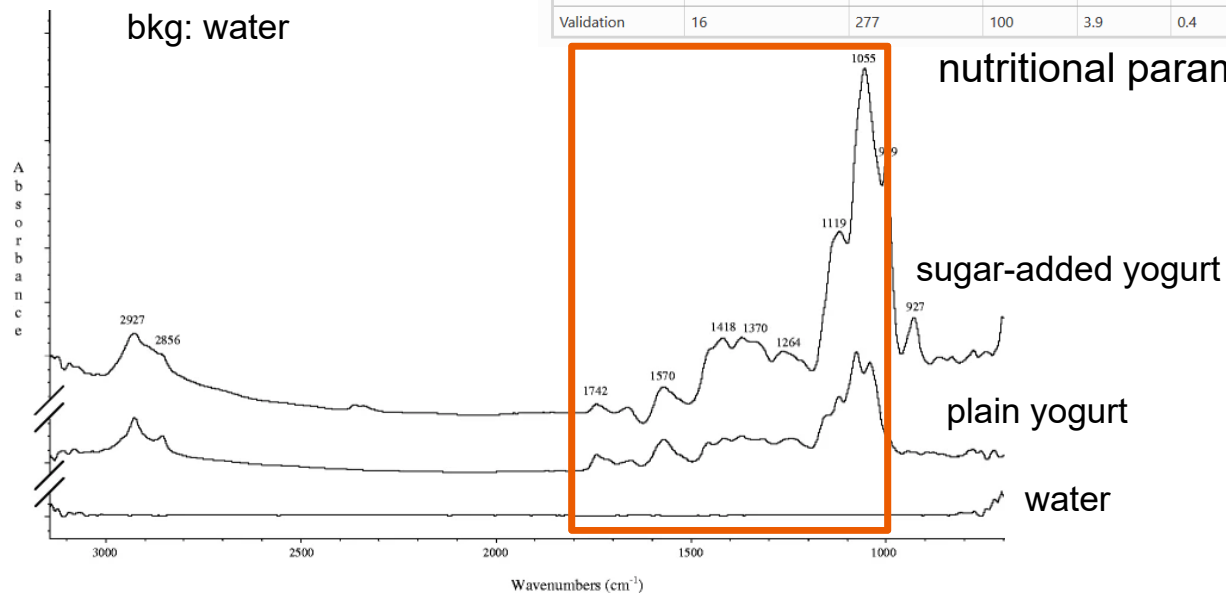


# Adsorbates by FTIR

- The carbonate ion




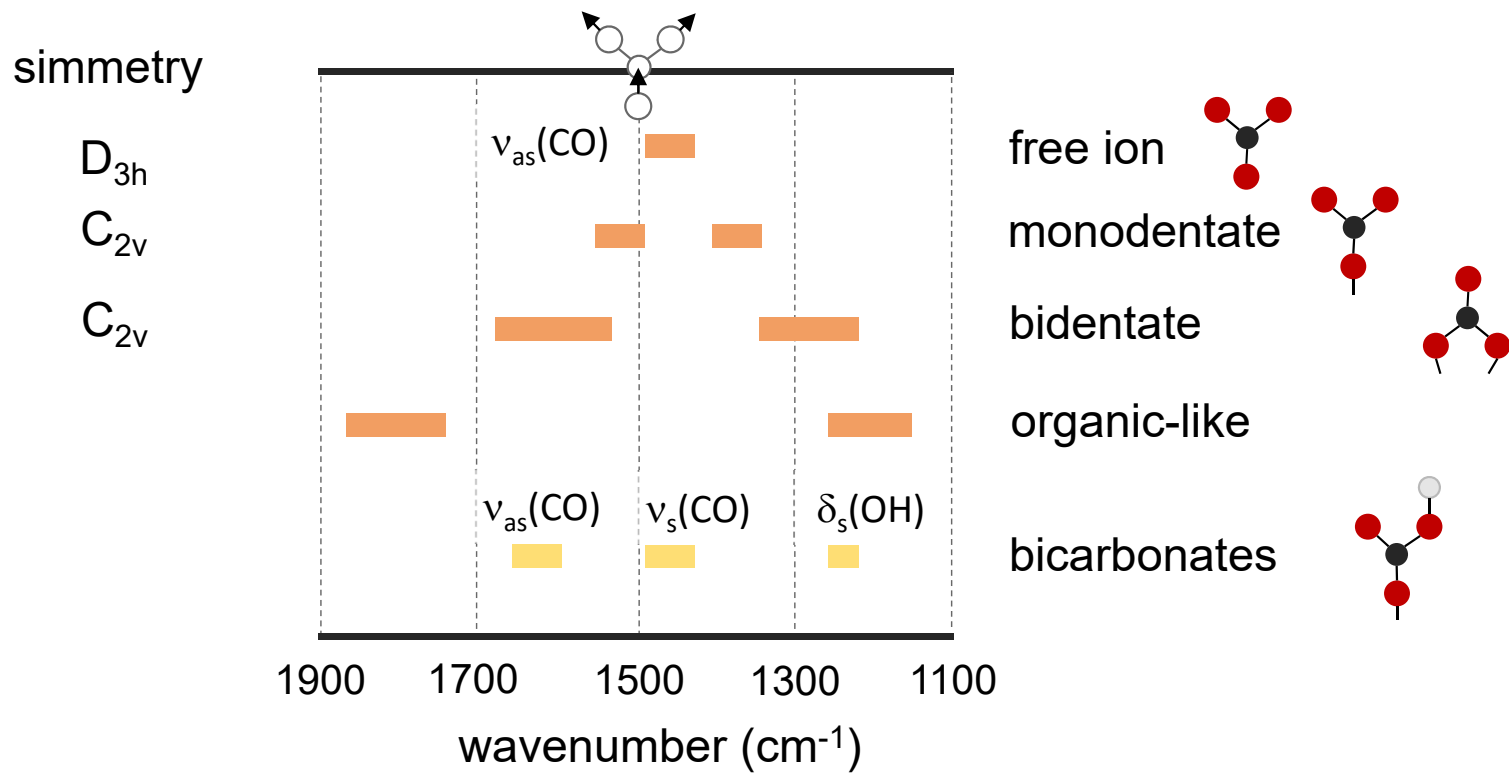


# Adsorbates by FTIR

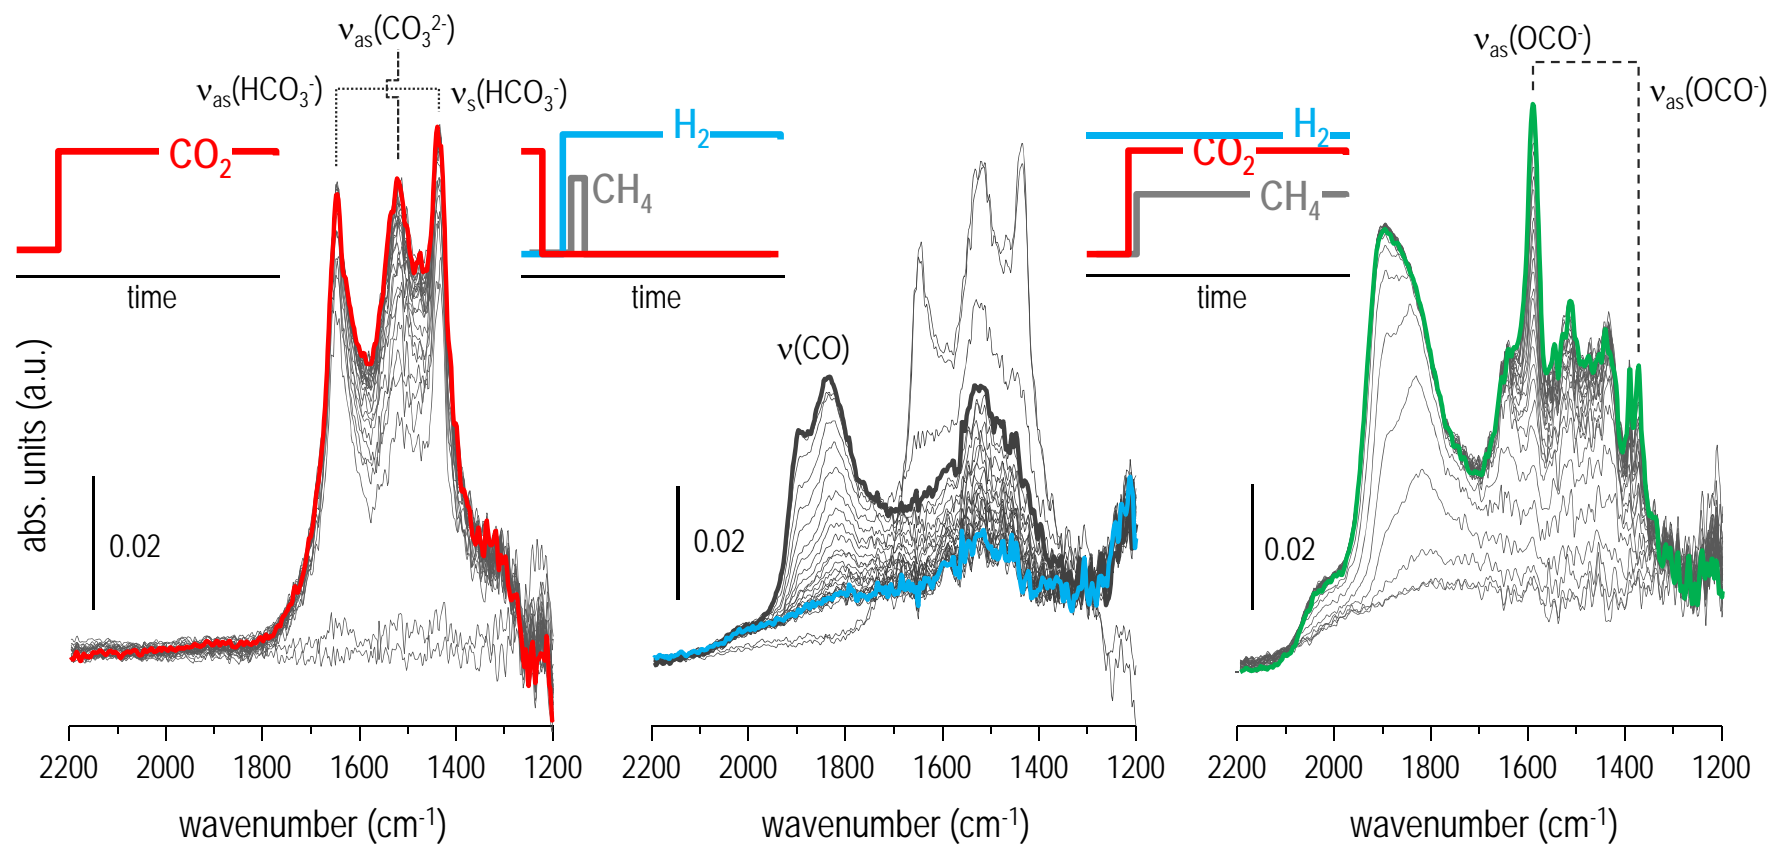




# Techniques, sample form, environment

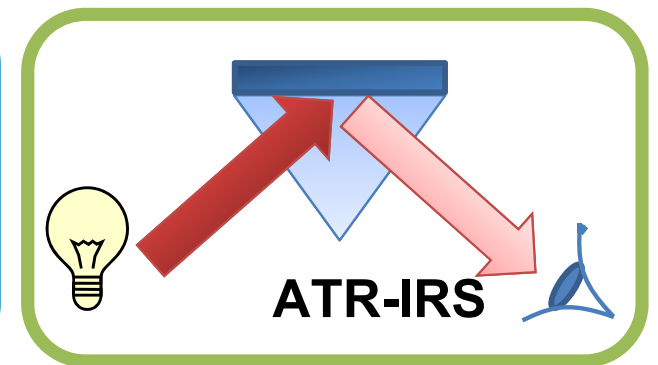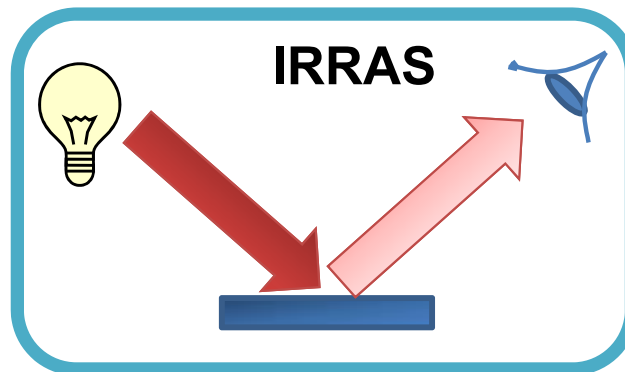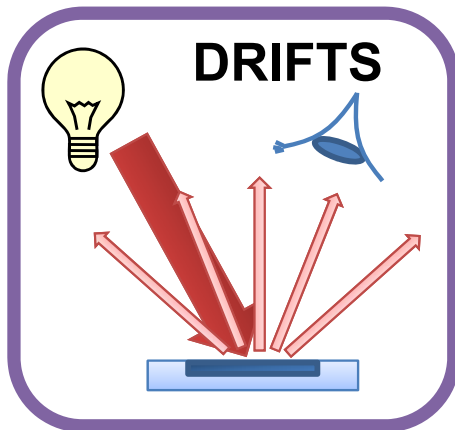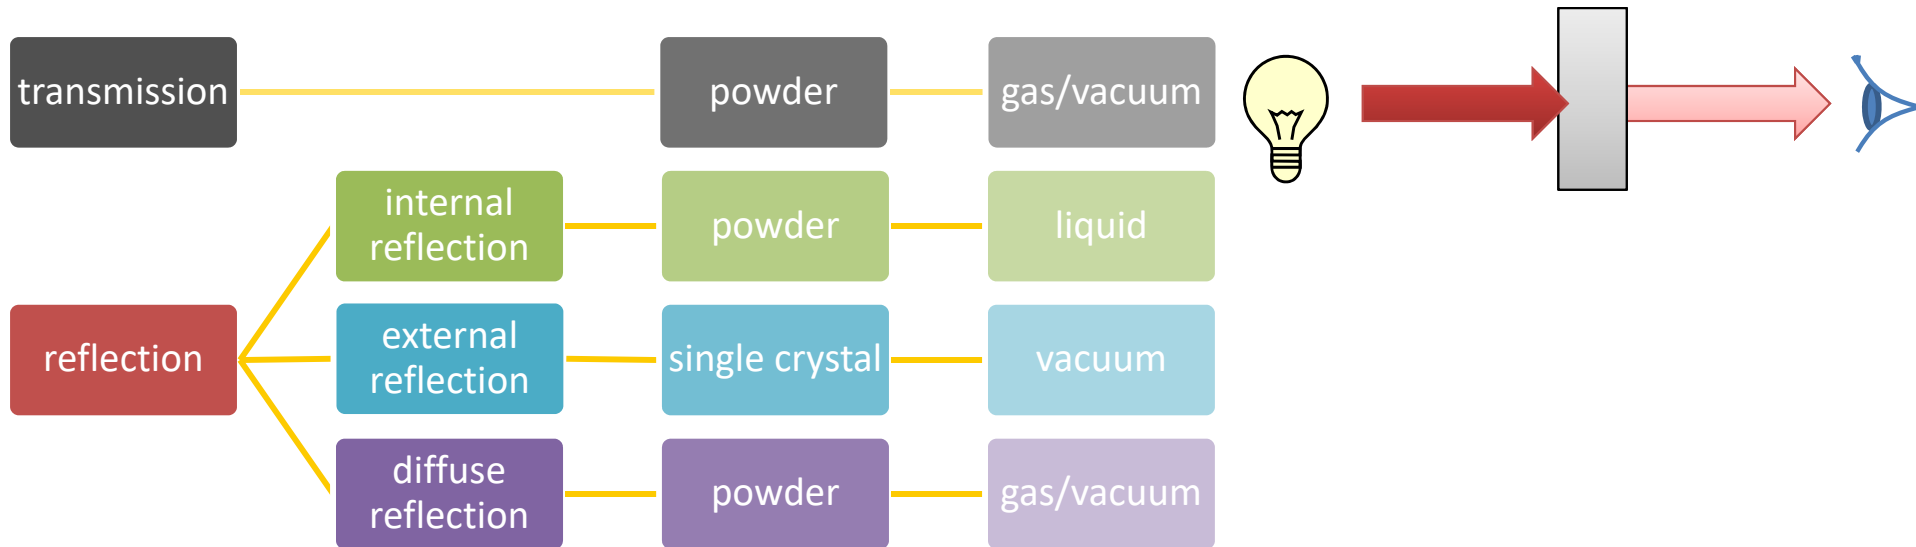

# Transmission

- Lambert-Beer law

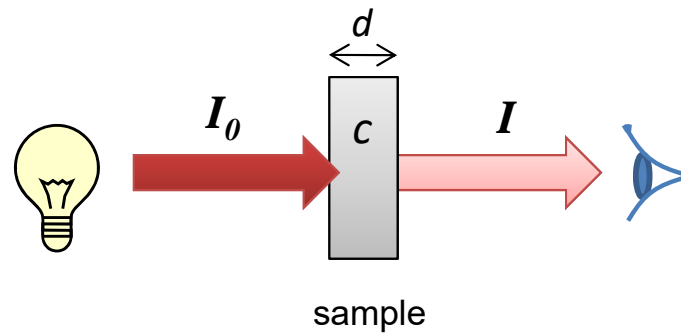

$$A = -\log(T) = -\log\left(\frac{I}{I_0}\right) = \varepsilon cd$$

**T**: transmittance, **A**: absorbance,  $\varepsilon$ : molar absorption (extinction) coefficient, **c**: concentration, **d**: path length

# Transmission

## ■ Solid samples

Large solid particles generally absorb too much IR light, therefore particles should be small and also special preparations are often necessary.

Most popular sample preparation methods (for mid-IR):

## ■ Alkali halide disk method

- Typically solid samples are diluted in KBr and ground
- Then pressurized to form a disk

## ■ Mull method

- Most common one is Nujol (liquid paraffin)
- Samples are ground and suspended in one or two drops of a mulling agent
- Followed by further grinding until a smooth paste is obtained


## ■ Film method

- By solvent casting or melt casting

**NOT FOR IN SITU/OPERANDO  
EXPERIMENTS**



# Transmission

- Sample preparation
  - self supporting wafers (few mg)
- Controlled exp. conditions
  - vacuum and controlled dosages
- Baseline
  - **slope** increases at high frequency (beam scattering increases with increasing frequency)
  - slope depends on particle size (very steep for powders with large particles, ca. 1  $\mu\text{m}$ )
  - $T$  @ 4000  $\text{cm}^{-1}$  is ca. 0 for large particle size oxides

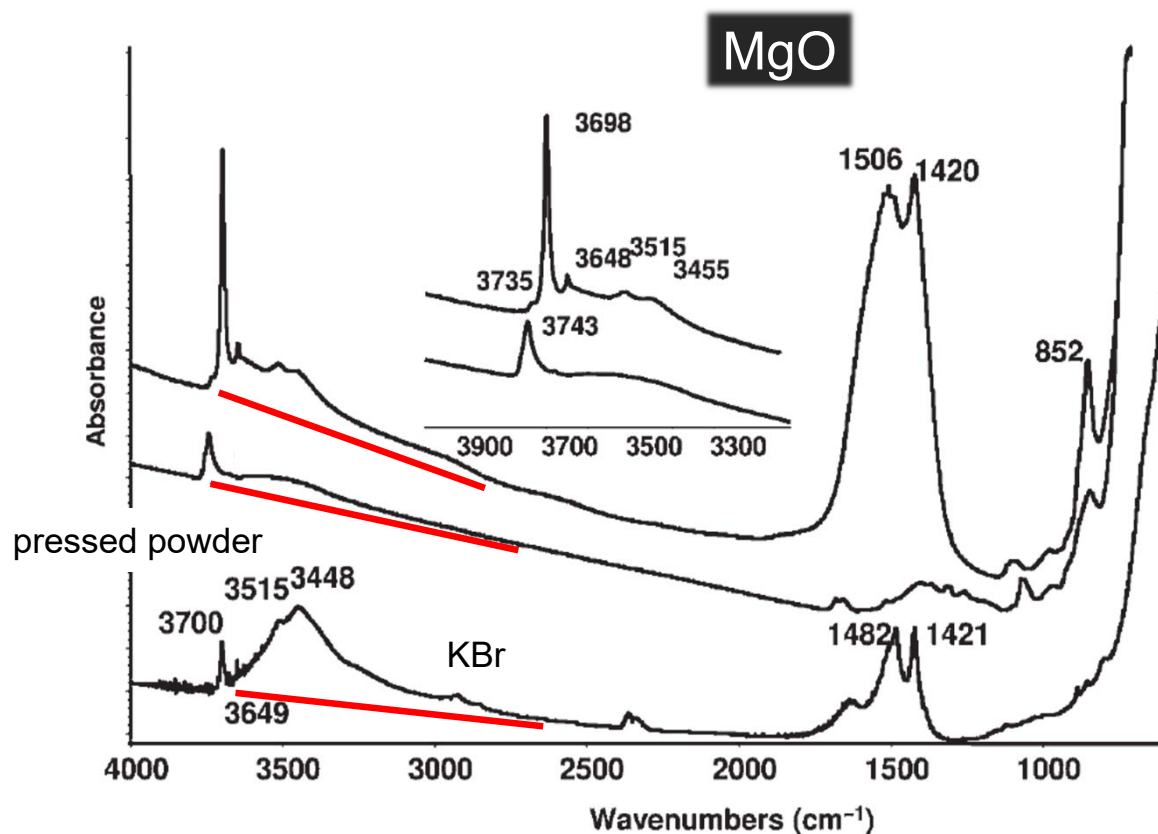

# Transmission

- Quantification | Molar absorption coefficient  $\epsilon$

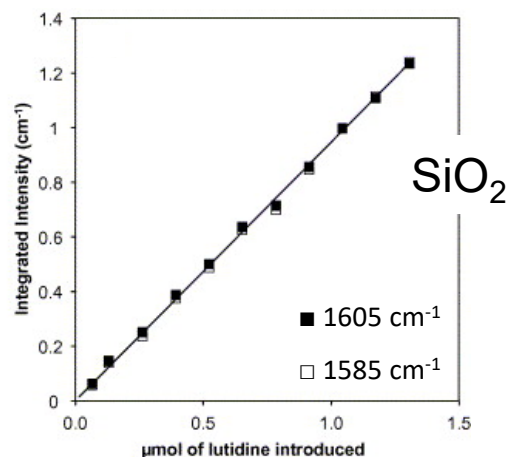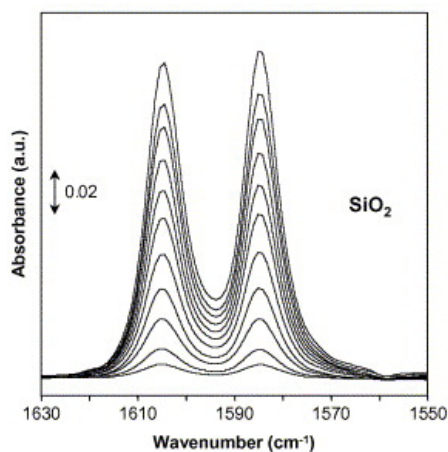

$$A = \epsilon \ell \frac{n}{S \ell}$$

$$A = \frac{\epsilon n}{S}$$


$$\epsilon = \frac{SA}{n}$$

$\epsilon$ , integrated molar absorption coefficient

$\ell$ , disc thickness (optical path)




$n$ , amount of adsorbed molecule

$S$ , disc area



# Diffuse reflection

- Combination of transmission and scattering/reflection

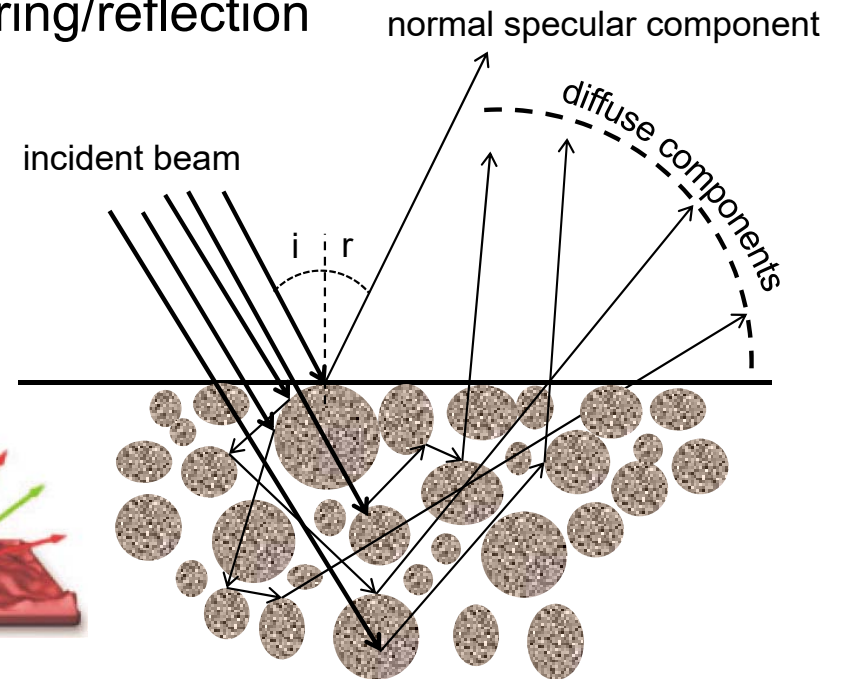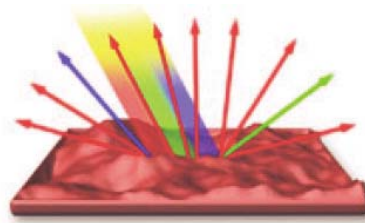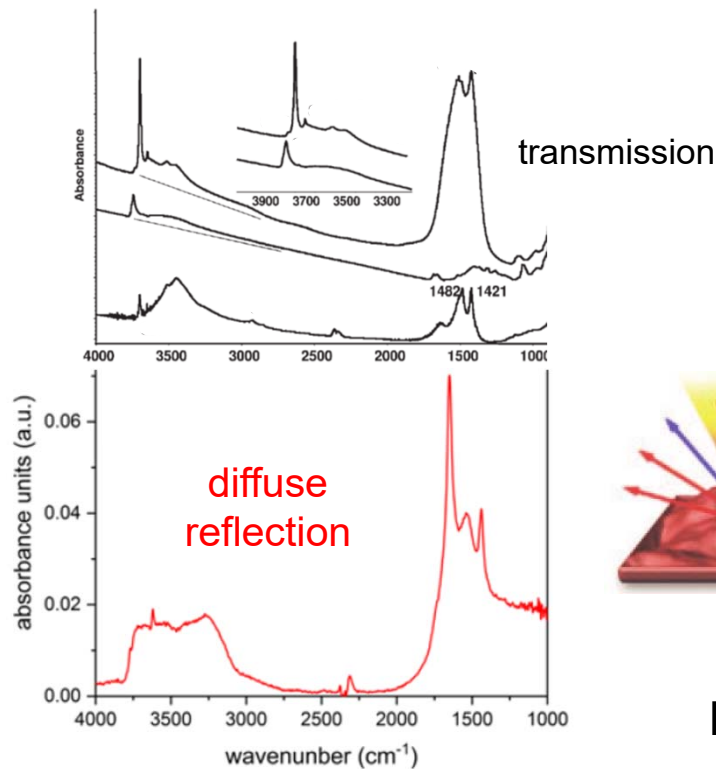

Reflectance increases by increasing scattering  
→ spectrum baseline is flat or even decreasing

# Diffuse reflection

- Qualitative analysis
  - very sensitive to surface species due to its diffuse reflective nature
  - the detected light is reflected multiple times at powder surfaces
- Quantitative analysis
  - can be very complicated
  - the spectra are largely influenced by various experimental parameters, e.g. particles shape and size, refractive index of particles, absorption characteristics of particles, and porosity of the powder bed
  - a popular method is to use the Kubelka-Munk (K-M) function to transform reflectance to a sort of absorbance (K-M) unit
  - solid (approximated) theory
  - applicability and accuracy for highly absorbing and non-absorbing samples is questionable

# Kubelka-Munk function

- Infinitely thick medium

$$K/S = (1-R_\infty)^2/2R_\infty$$

K, absorption coeff.


S, scattering coeff.

- Adsorbate on infinitely thick medium

$$(K+\varepsilon C)/S = (1-R)^2/2R$$

$$F(R) = J(1/R - R_\infty) = 2\varepsilon C/S$$

Kubelka-Munk function

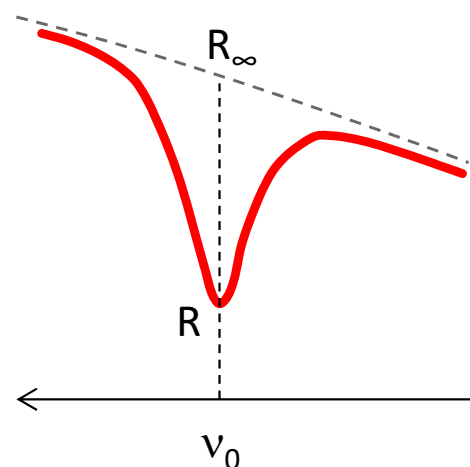





$$J = \frac{R_\infty - R}{R_\infty}$$

optical length ( $d$  in L-B Law) much larger than in transmission → more sensitivity



# Diffuse reflection

- Reflectance or Absorbance?

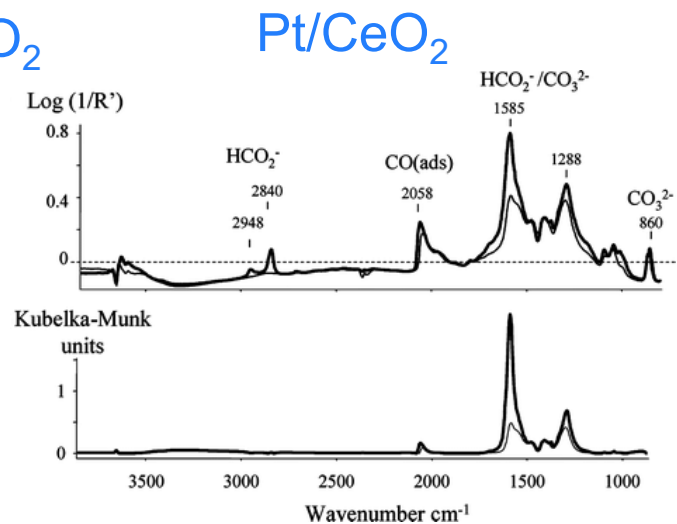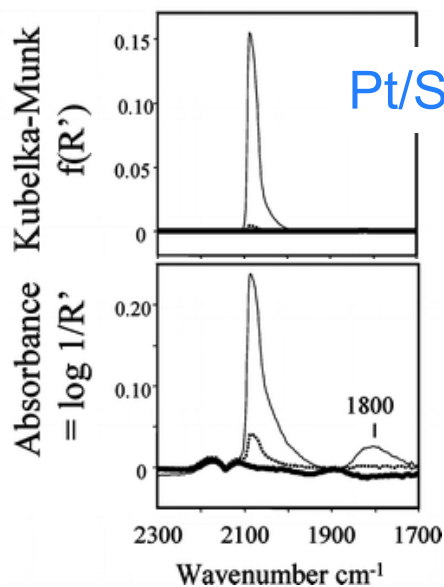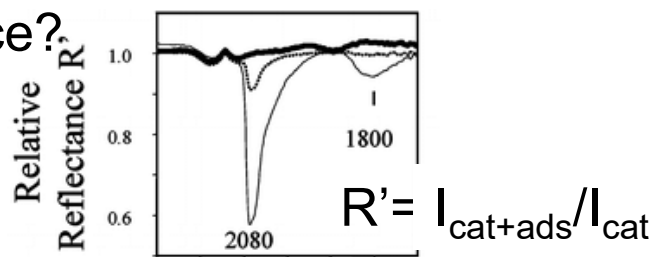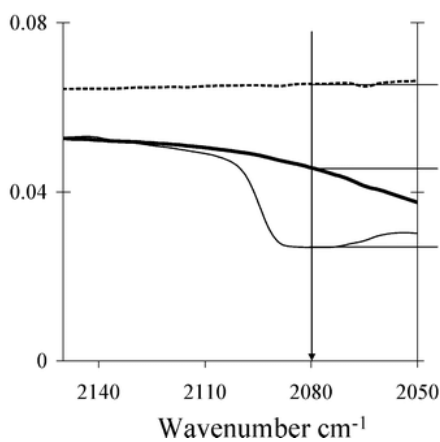


# Diffuse reflection vs Transmission

- Advantages of diffuse reflection
  - easier sampling
  - applicability to powders that scatter too much in transmission, assuming the surface area is sufficiently high to detect surface
  - vibrations with a sufficiently high signal-to-noise ratio
  - slightly lower sensitivity to bulk conduction phenomena, because of a higher surface-to-bulk sensitivity ratio
  - ideally suited for in situ/operando studies
- Disadvantages of diffuse reflection
  - less obvious optical setup
  - work in flow rather than in vacuum
  - more difficult sample activation (i.e. water removal from highly porous materials)


## Diffuse reflection vs Transmission

- Comparison between techniques with different sensitivity (bulk/surface) should be careful
- DRIFTS more sensitive than TIRS
- Band assignment depends on surface sensitivity of the technique

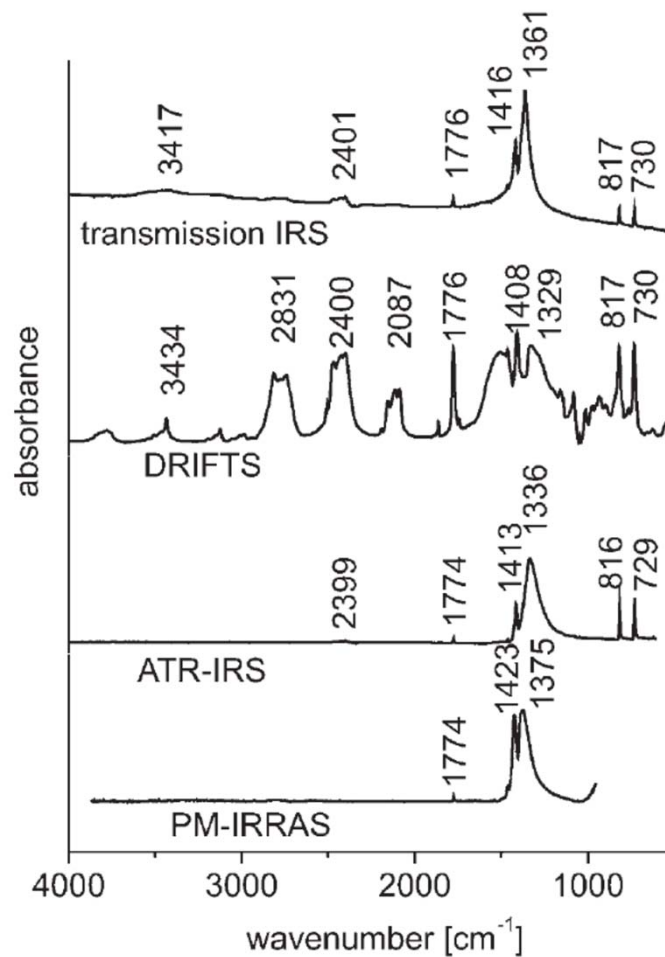


# Diffuse reflection

- Typical mirror unit, sample holder and in situ cell

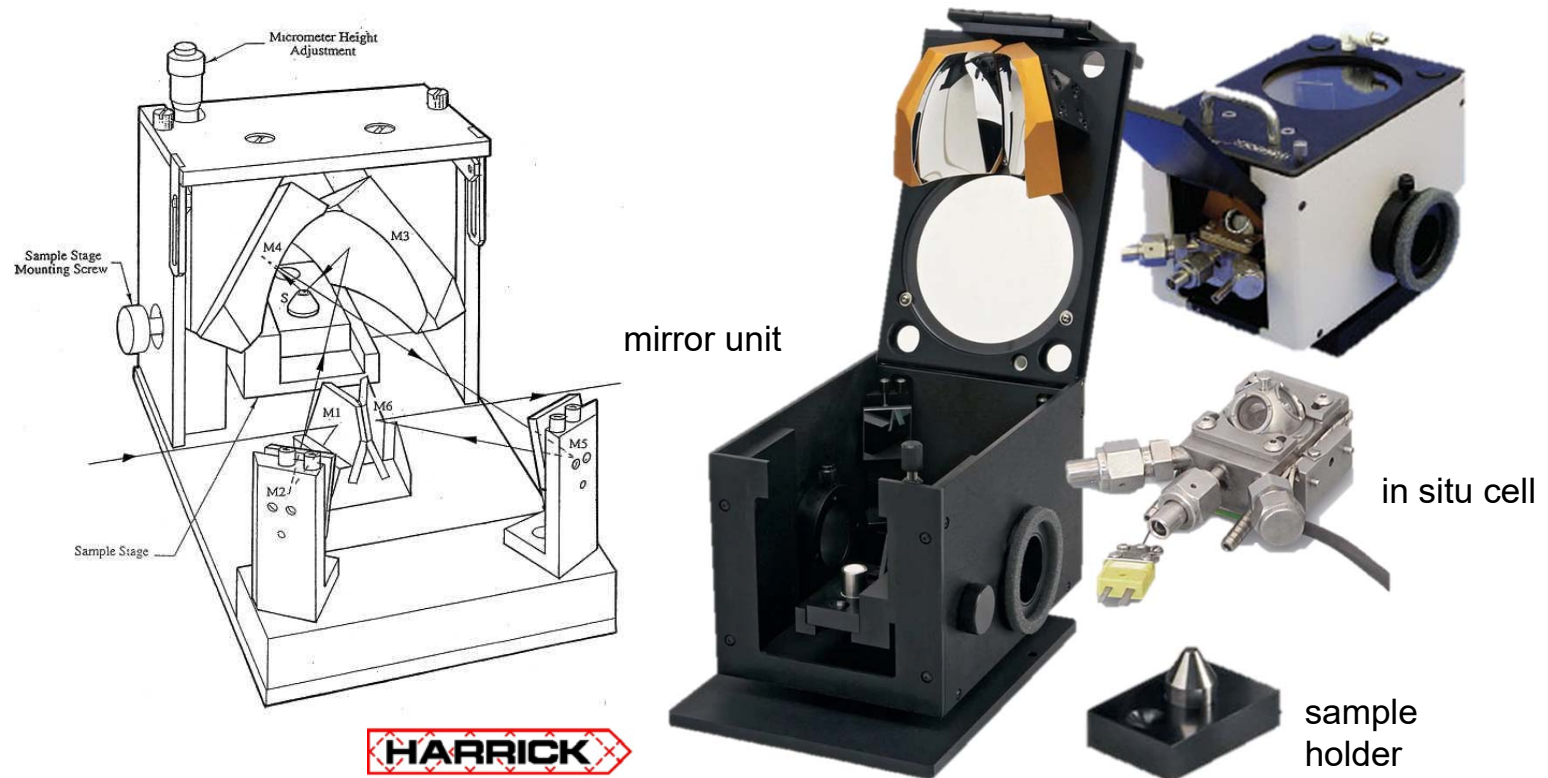

Harrick Scientific | Praying Mantis

# Attenuated total reflection

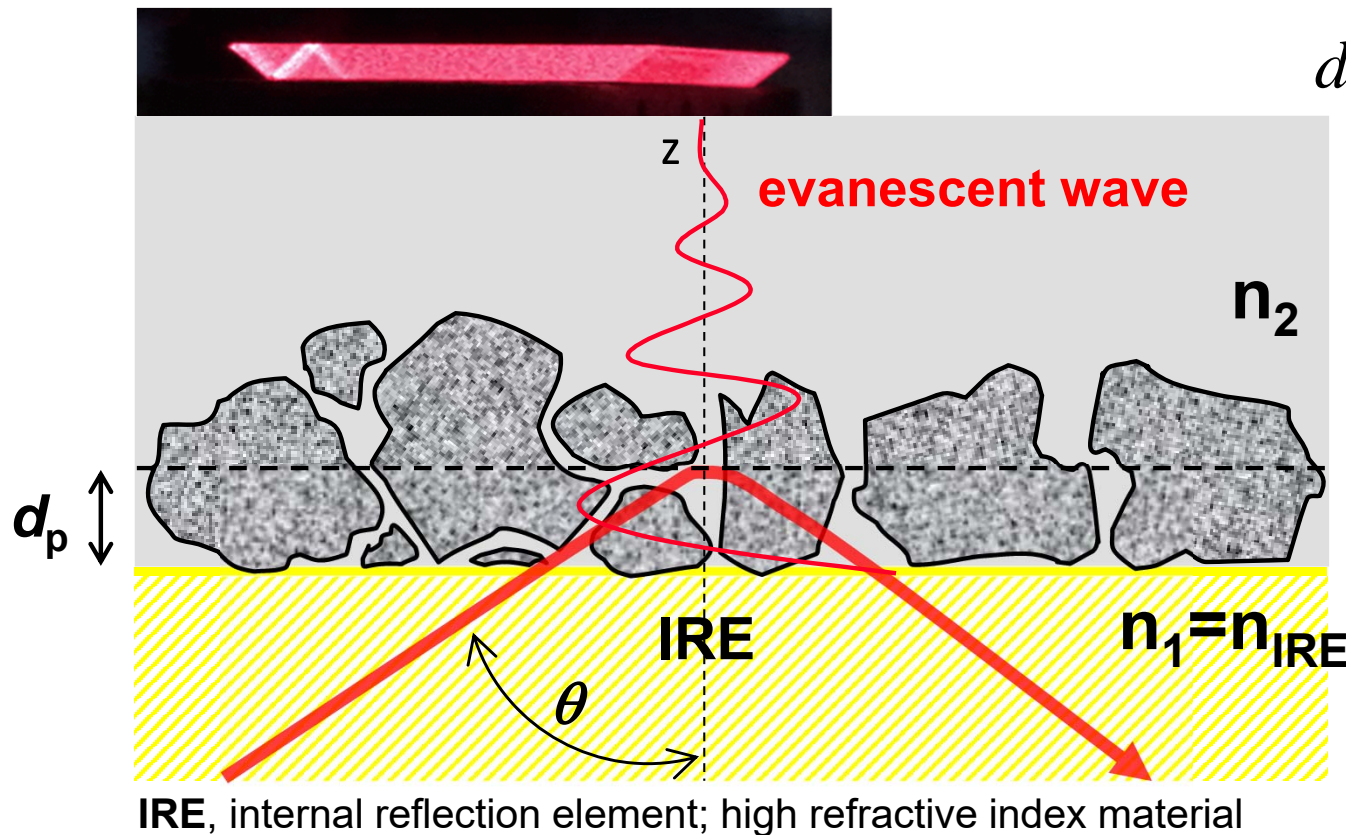

$$d_p = \frac{\lambda_1}{2\pi \sqrt{\sin^2 \theta - n_{21}^2}}$$

$\theta$ : angle of incidence




$$\lambda_1 = \frac{\lambda}{n_1} \quad n_{21} = \frac{n_2}{n_1}$$

$d_p$ : penetration depth  
the distance from interface where the electric field has decayed to  $1/e$  of its value  $E_0$  at the interface


IRE, internal reflection element; high refractive index material

# Attenuated total reflection

- Sample preparation
  - sample deposition on IRE from aqueous slurry
  - dry in air

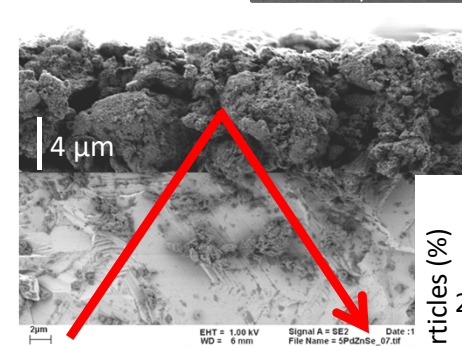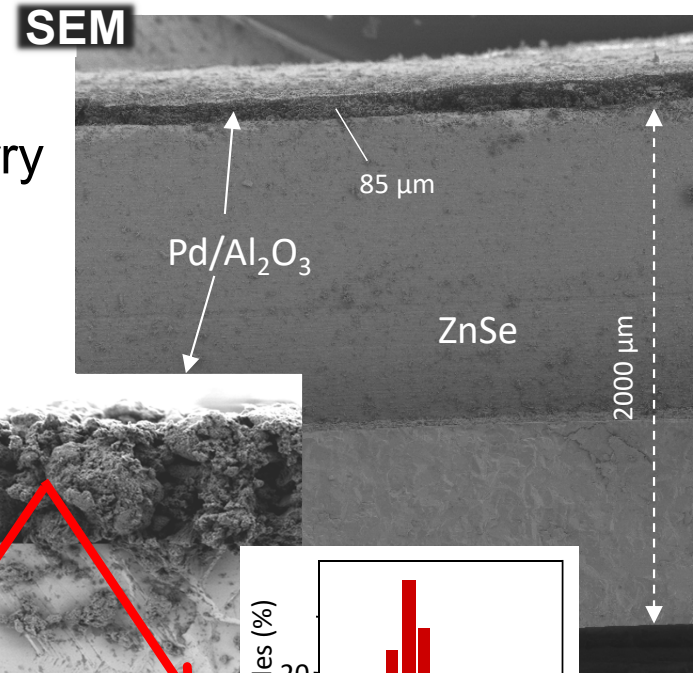
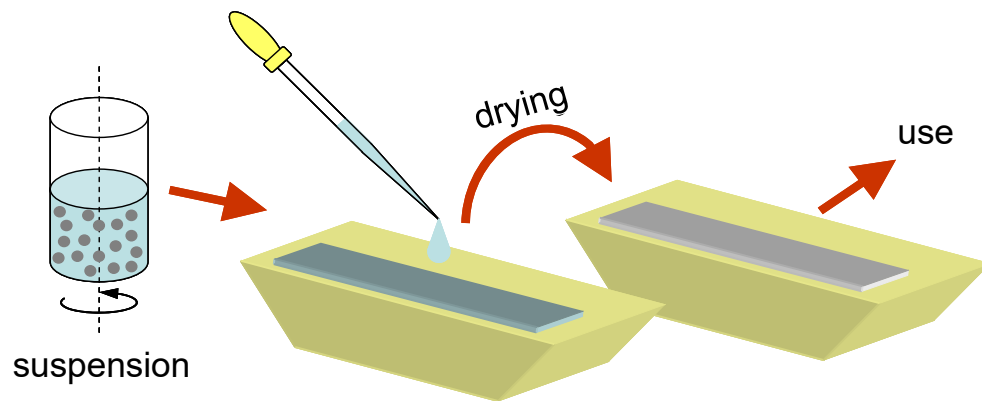


IR

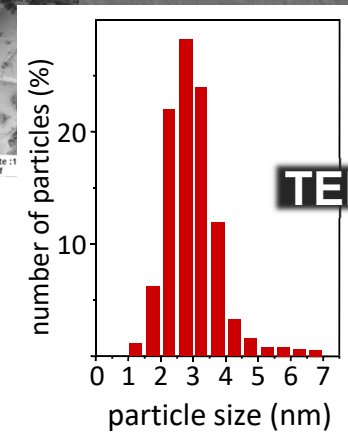



TEM

# Attenuated total reflection

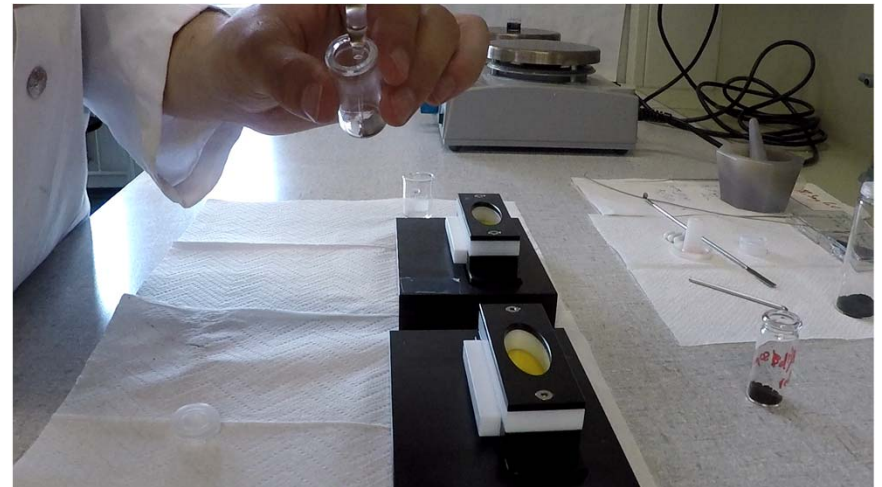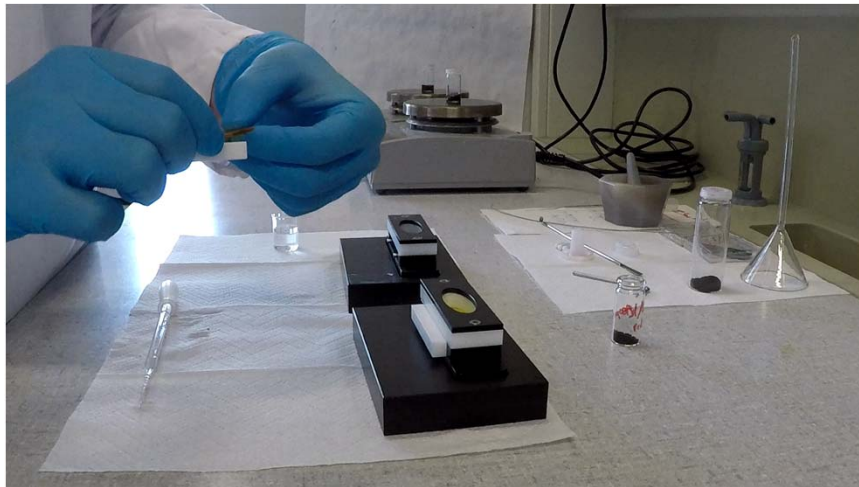

# Attenuated total reflection

- Stable films needed for in situ investigations

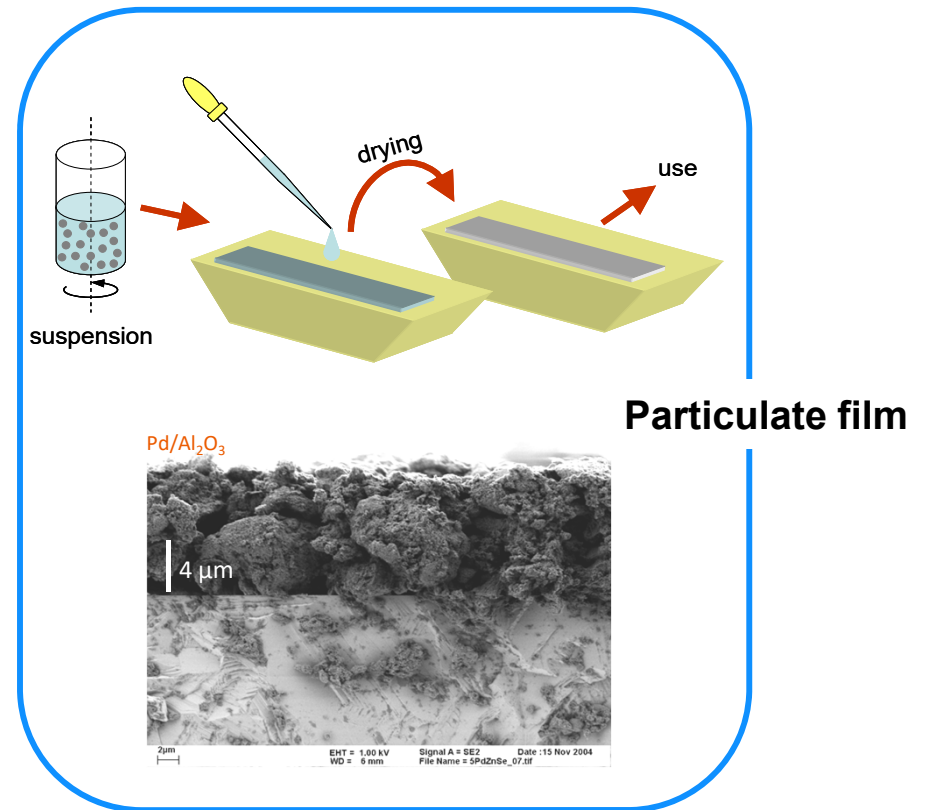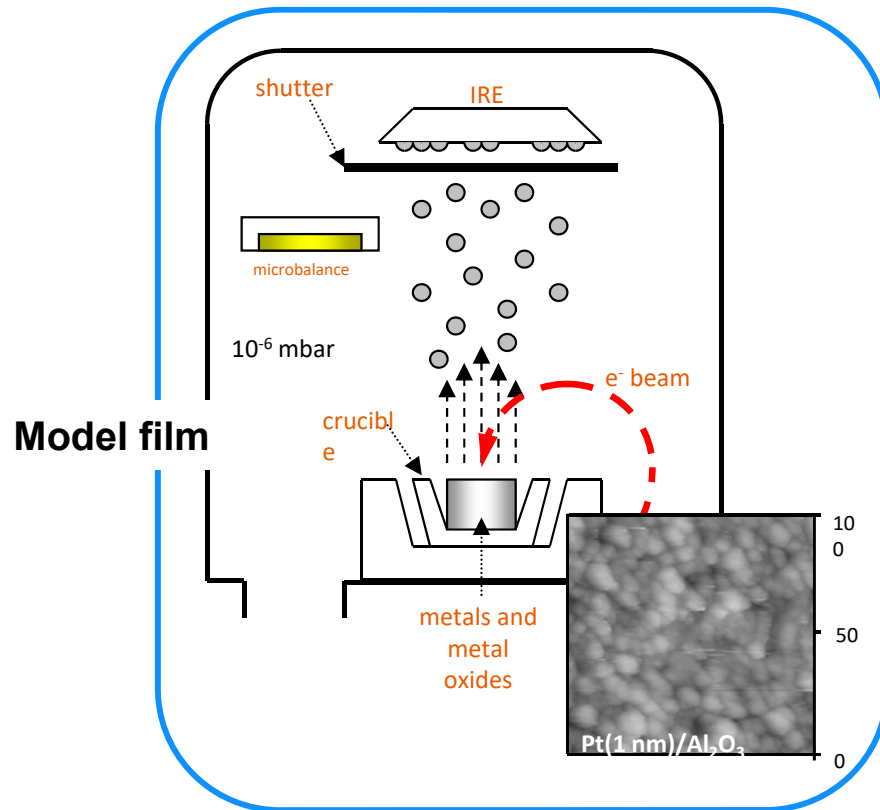




## Materials for internal reflection elements


Material	Useful range / $\text{cm}^{-1}$	n	$d_p$	Properties
ZnSe	20000-700	2.43	long	soluble in strong acid; usable up to ca. 300°C
Ge	5000-900	4.02	short	good chemical resistance; hard and brittle; becomes opaque at 250°C
Si	9400-1500; 350-FIR	3.42	short	excellent chemical resistance; hard; usable up to ca. 300°C
KRS-5 (Thallium bromoiodide)	14000-330	2.45	long	toxic; slightly soluble in water and soluble in base; usable up to ca. 200°C

# Attenuated total reflection

- The meaning of  $d_p$  and  $n_{IRE}$

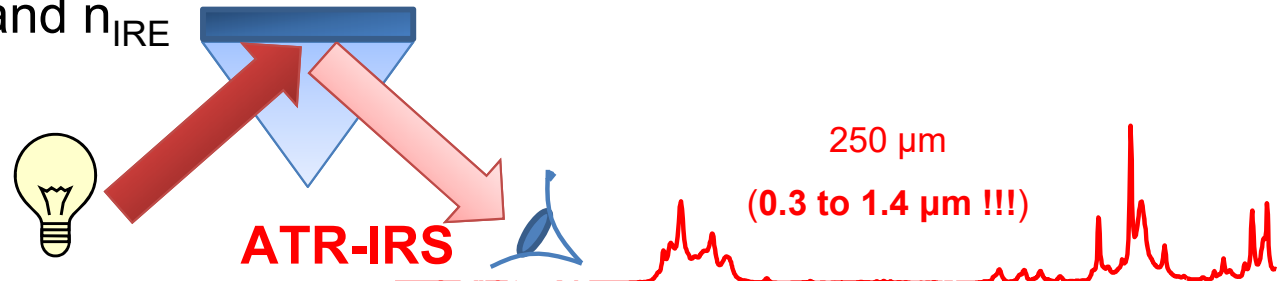


same spectrum as in transmission but with much smaller sample thickness

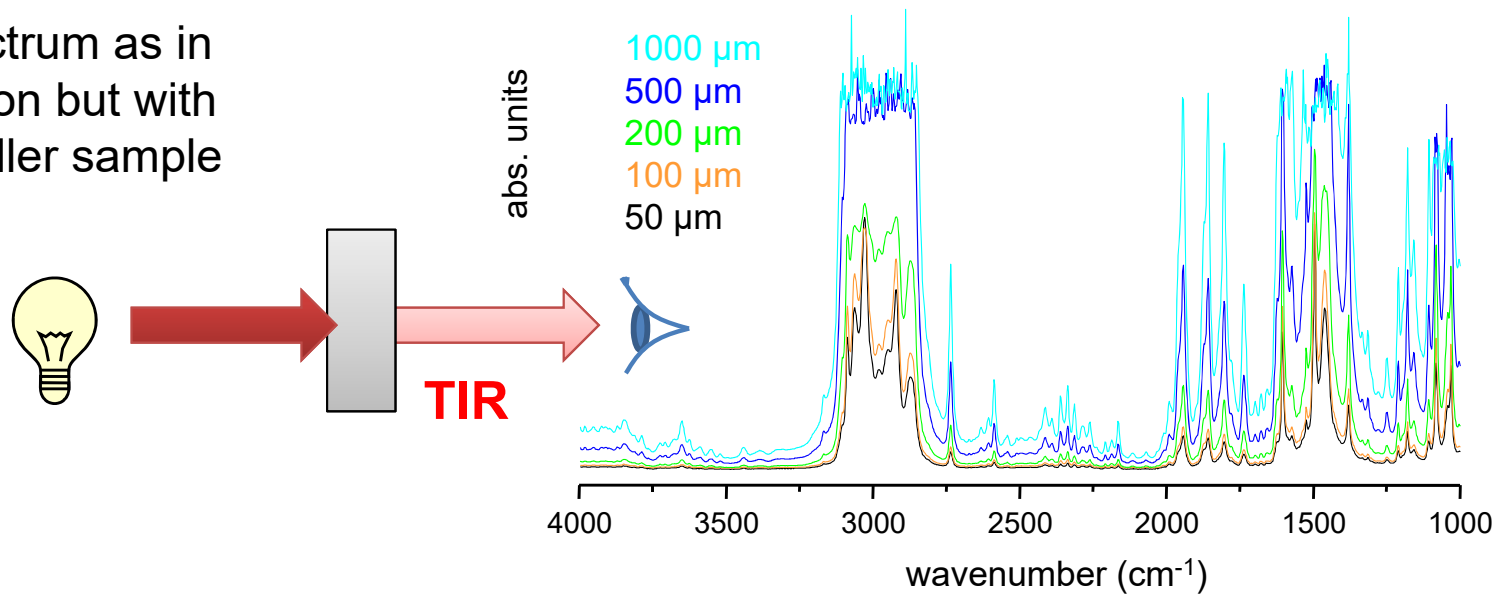


# Attenuated total reflection

- The meaning of  $d_p$  and  $n_{IRE}$

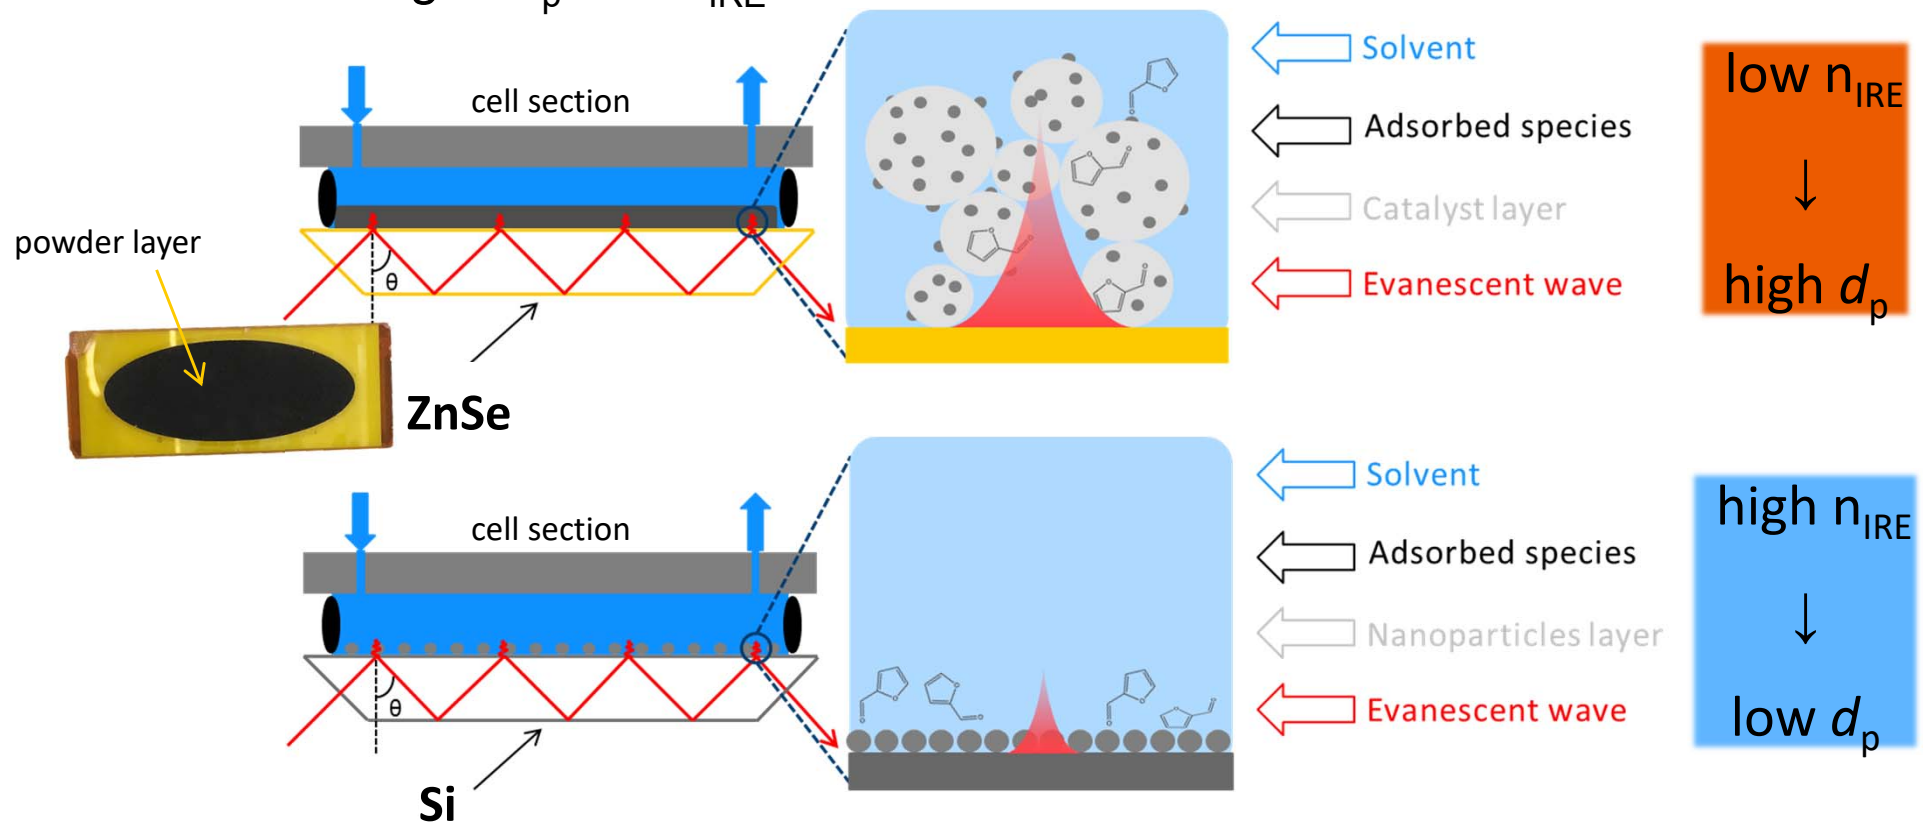

# Attenuated total reflection


- Solid (powders, crystals, foils, plates, seeds...) and liquid samples
- Ex situ
  - structure assignment
  - identification
  - quality control

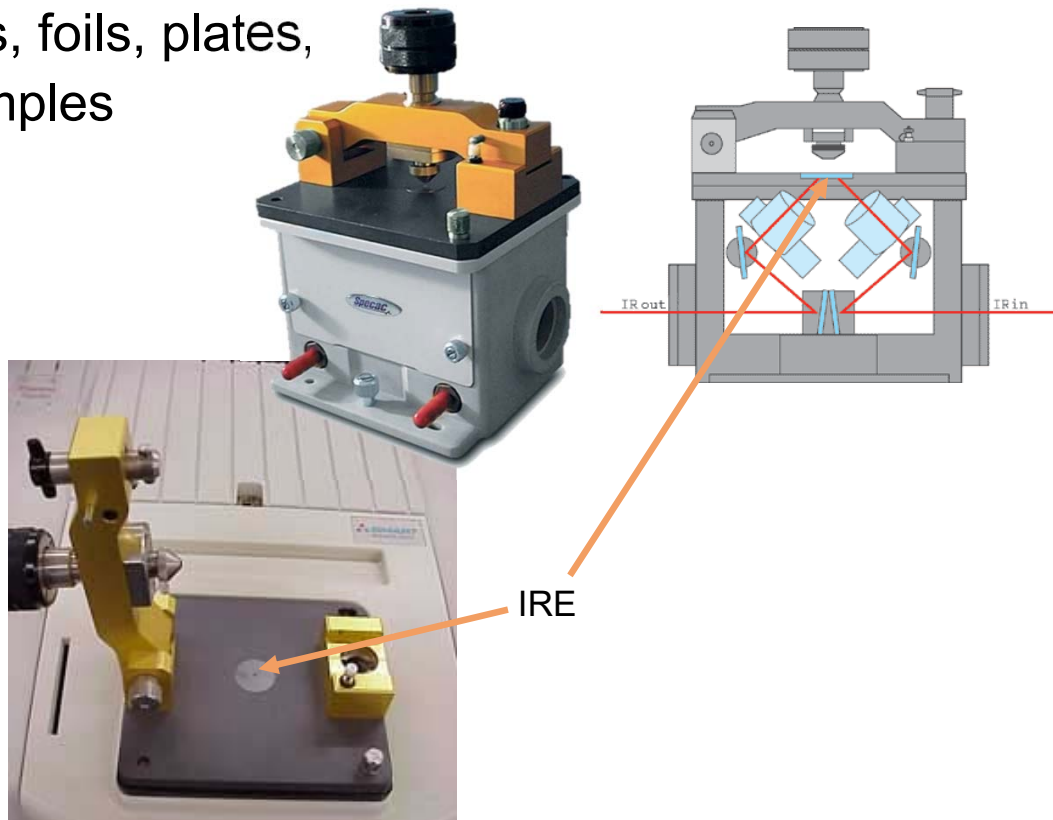

# Attenuated total reflection



- Solid (powders, crystals, foils, plates, seeds...) and liquid samples
- Ex situ

- In situ/operando
  - only liquids
  - suspensions
  - solid in contact with liquid

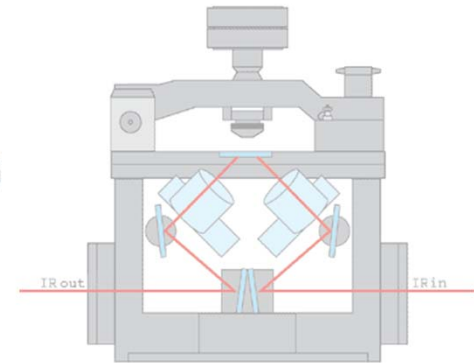


# Attenuated total reflection

- Cell mounting

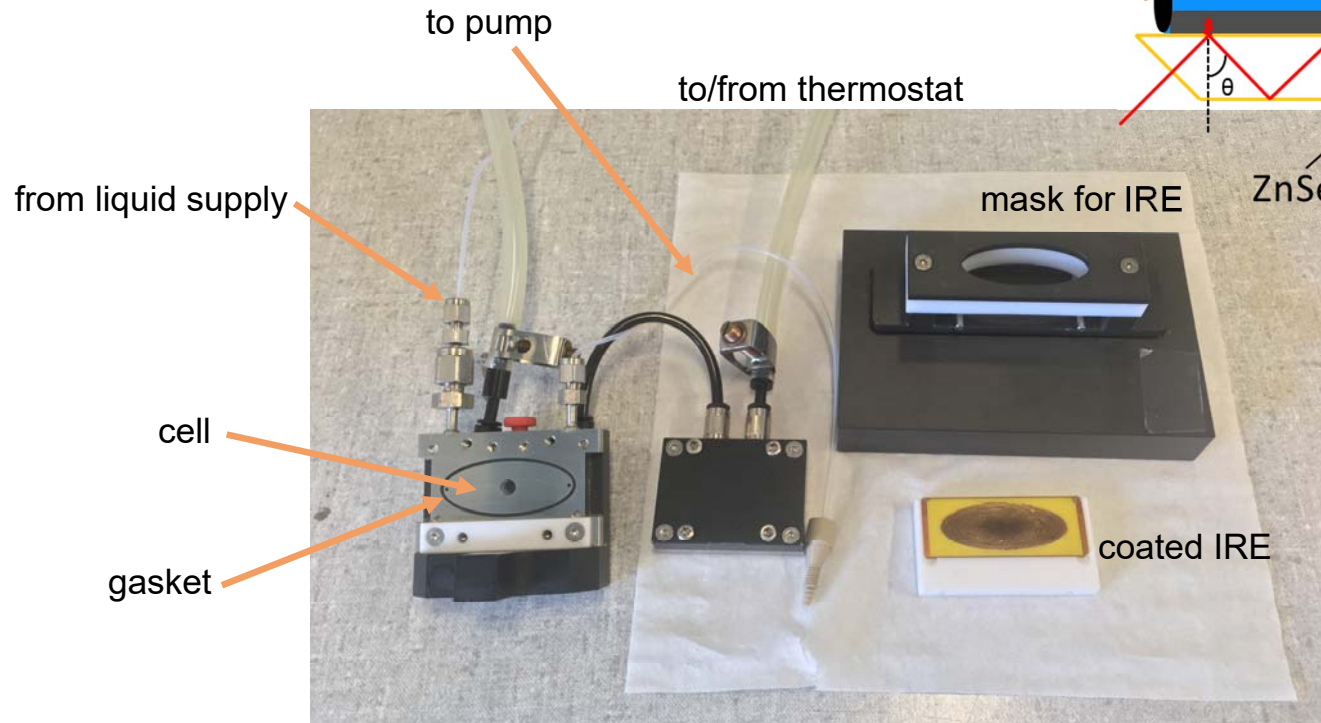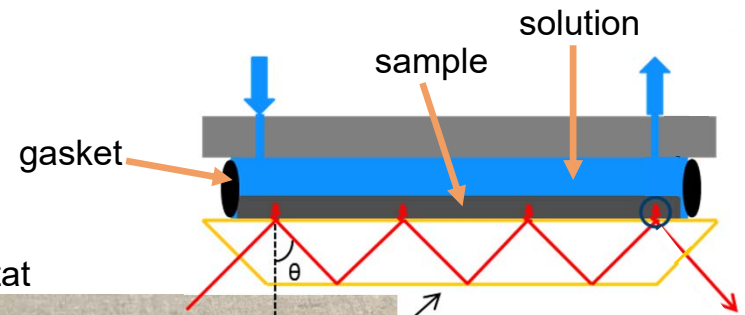


# Attenuated total reflection


- Sample compartment

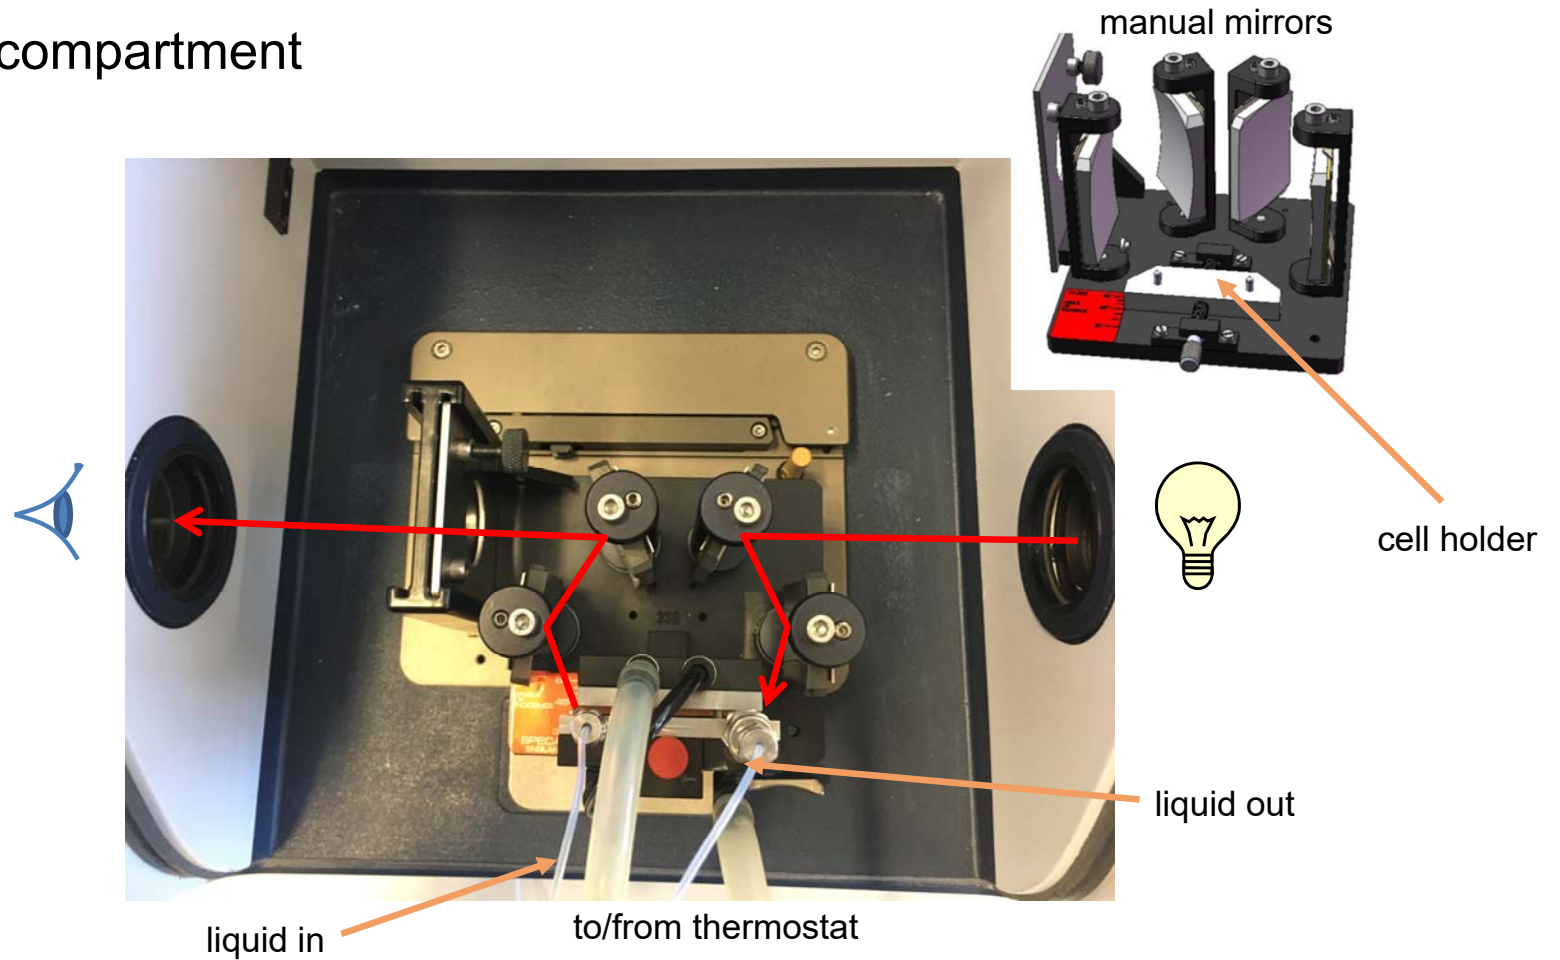

# Knoevenagel condensation


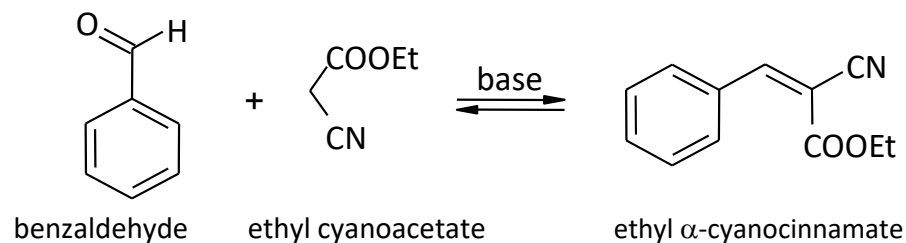


- $\gamma$ -aminopropyl modified  $\text{SiO}_2$  (APS- $\text{SiO}_2$ )
  - 1.5 mmol/g  $\text{NH}_2$
  - 202  $\text{m}^2/\text{g}$
  - deposited on ZnSe from
    - $\text{CCl}_4$  slurry
    - toluene/PE slurry prep. 80°C
    - dried in *vacuum*
- toluene, 60°C

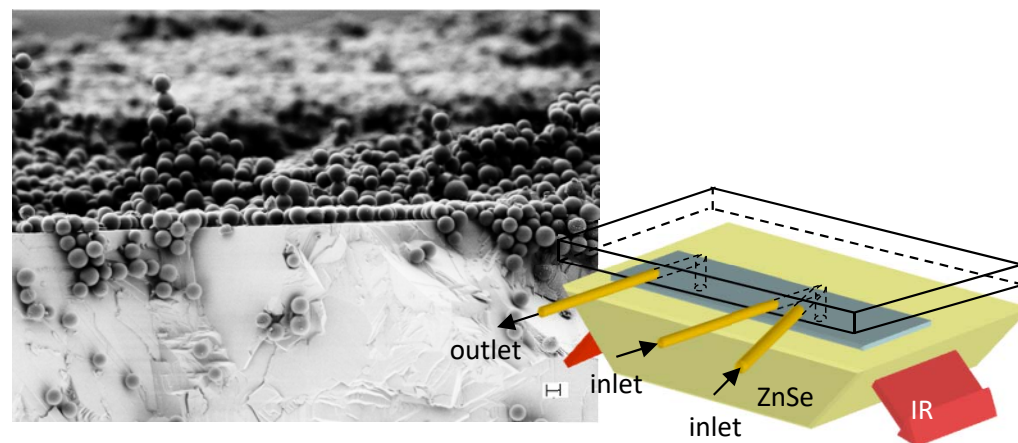




# Knoevenagel condensation

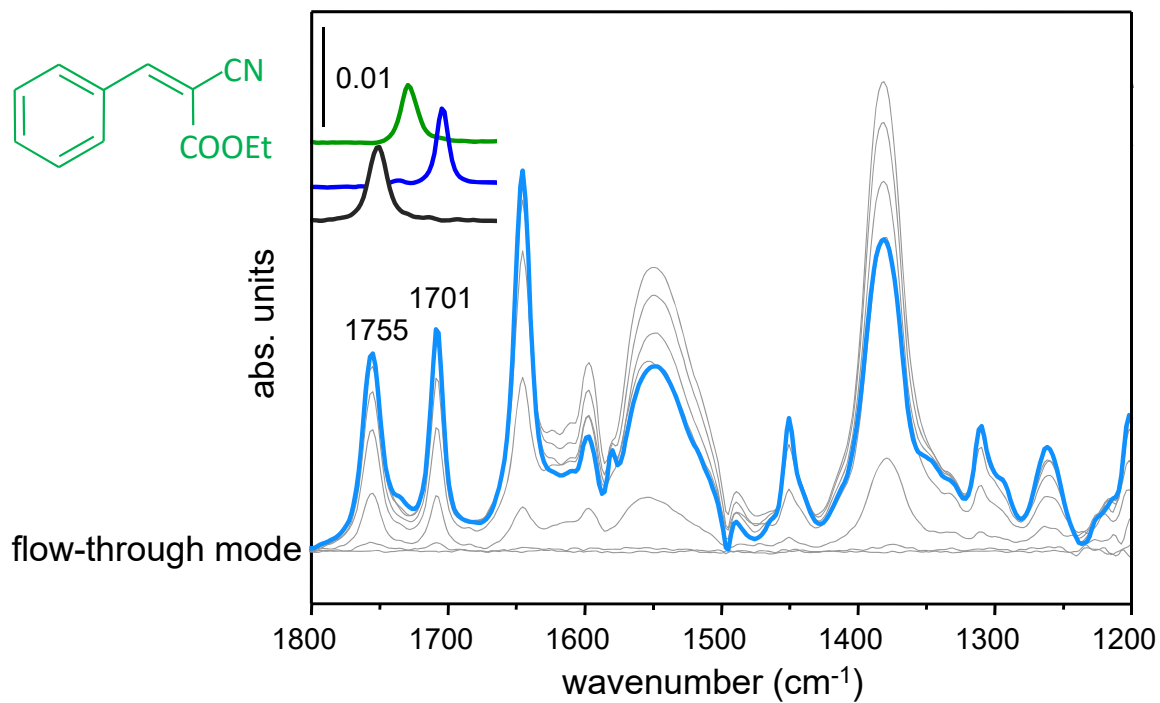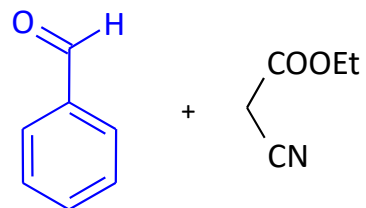

toluene, 60°C, 20 mM



# Knoevenagel condensation

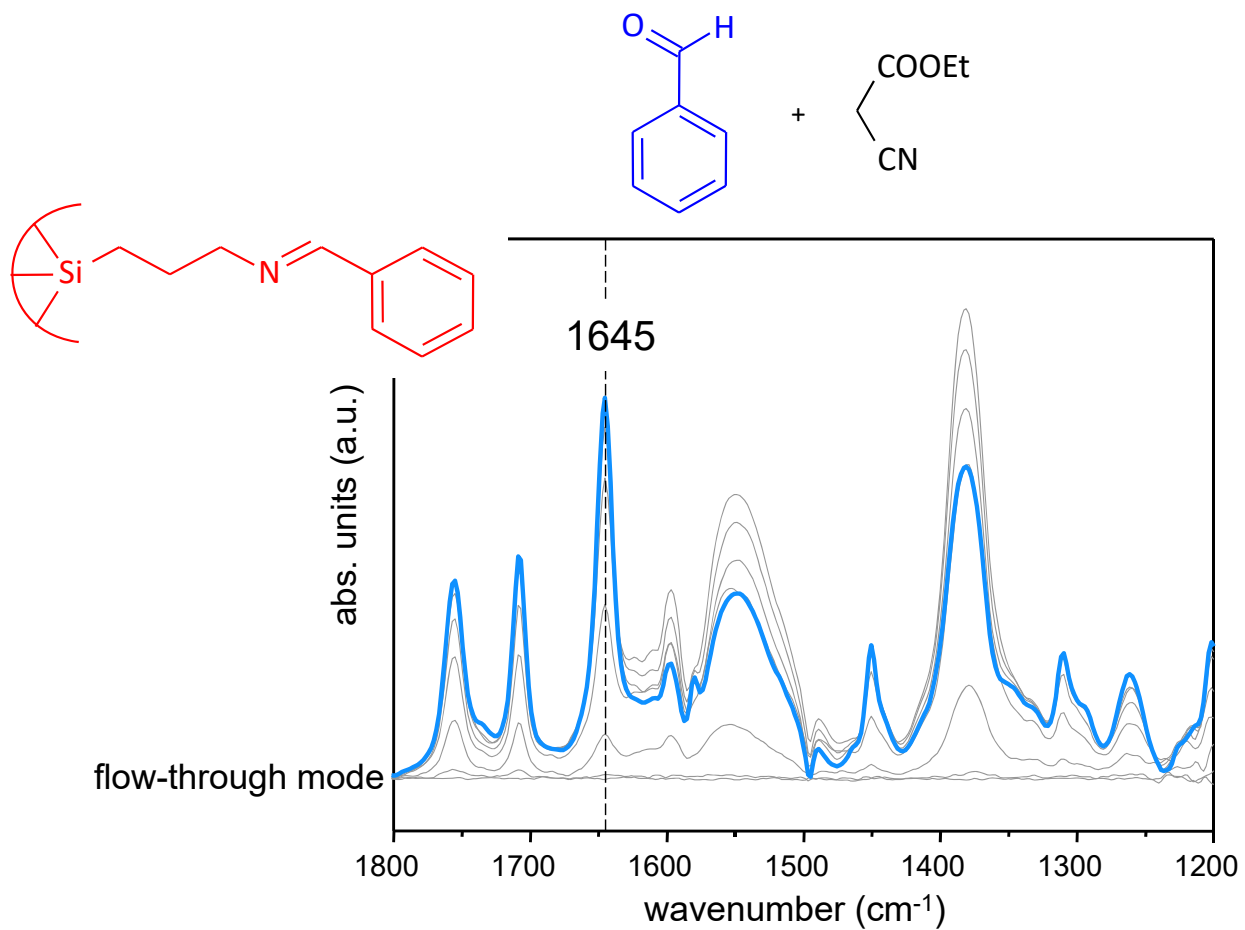

toluene, 60°C, 20 mM


# Knoevenagel condensation

- Consecutive dosage of reactants
- Time dependence

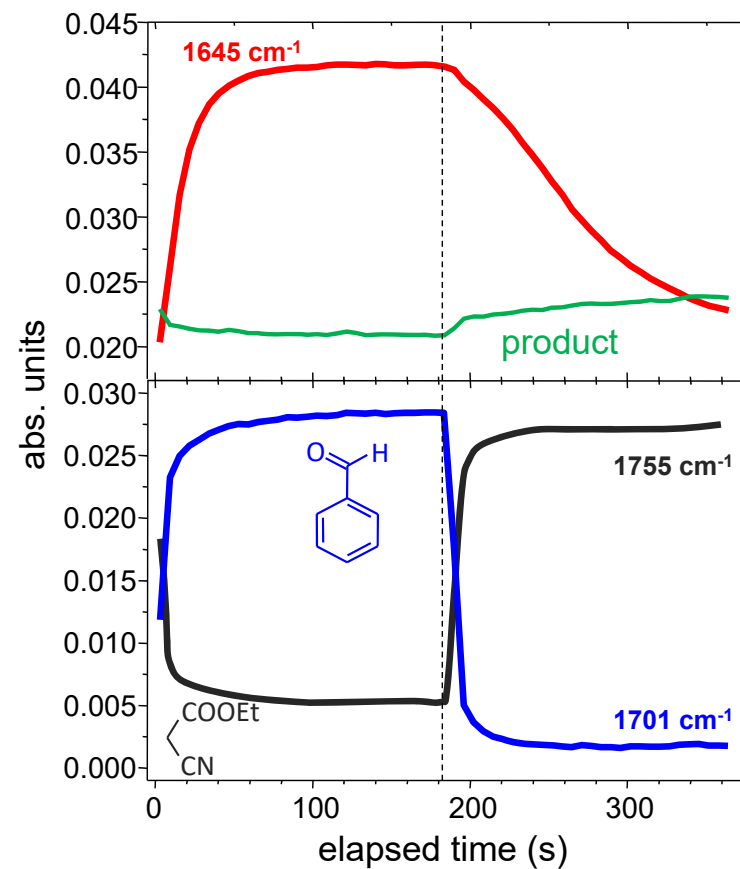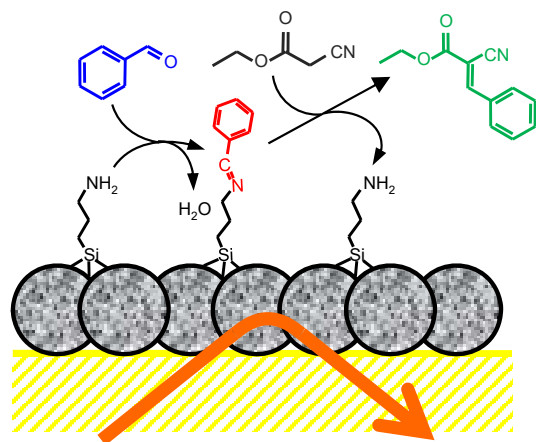


# Knoevenagel condensation

- Stopped-flow mode

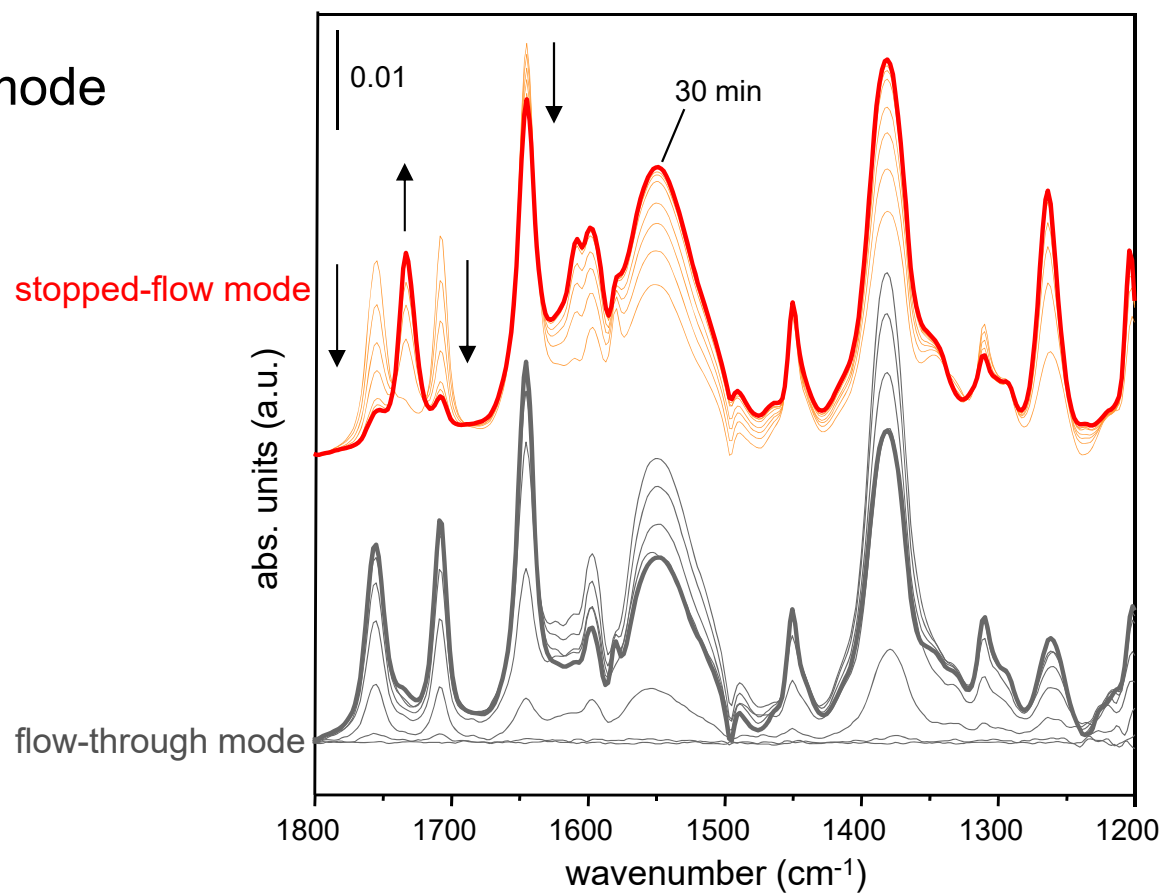


toluene, 60°C, 20 mM

# Knoevenagel condensation

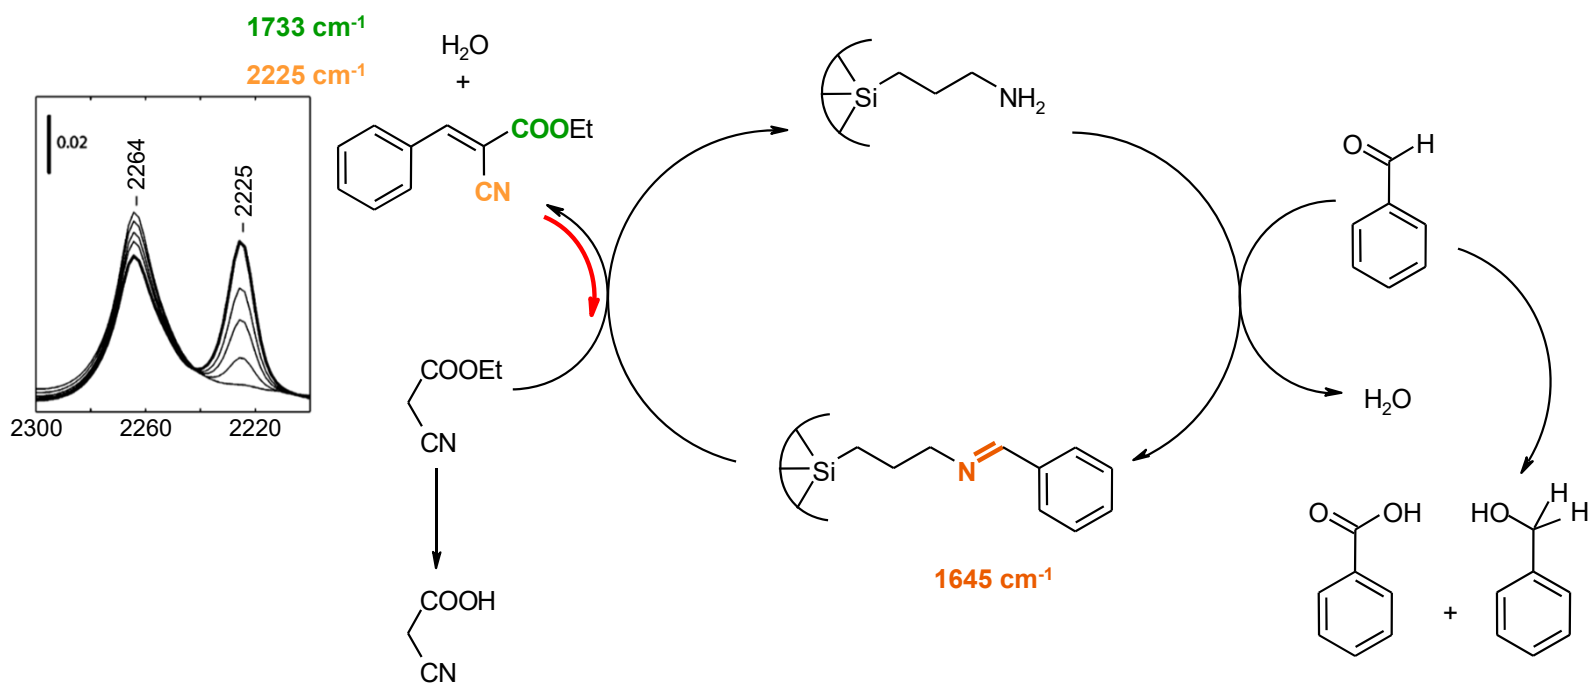

# CO adsorption

## Blyholder model

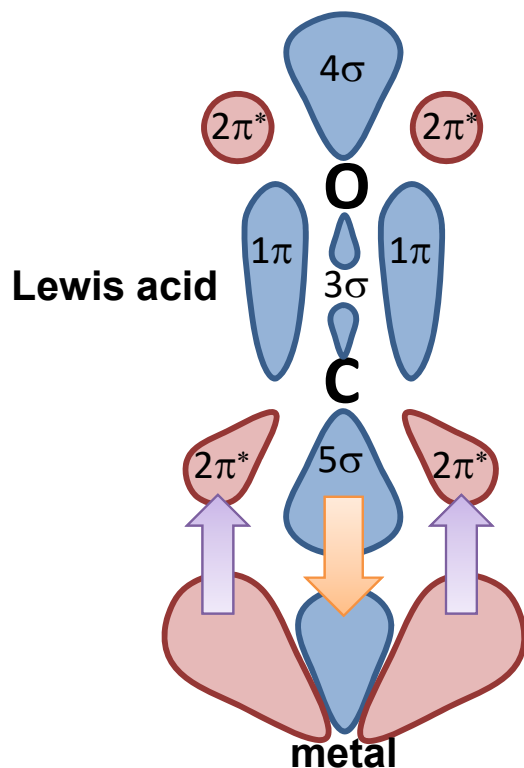

### Donation


CO donates electrons from the s orbital to the metal

### Back-donation (BD)

metal donates electrons back to the anti-bonding  $\pi$  orbital of CO

- Low CO coverage:  $\nu_{\text{CO}}$  depends on the geometry of **adsorption site** (face order: **terrace – corner – edge**) – **BD is strong**
- High CO coverage:  $\nu_{\text{CO}}$  depends on **dipole-dipole interactions** – **BD is weak**


# CO adsorption

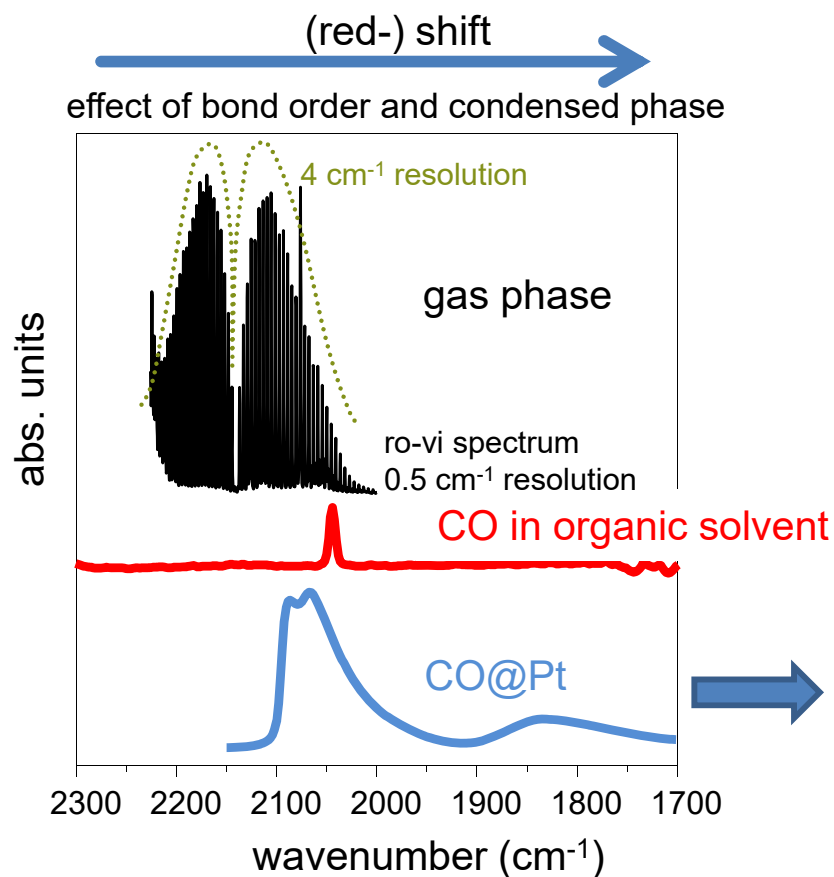




**Adsorbate**  
assignments on powders  
by comparison with  
reference exps. in UHV  
(single crystals)

# CO adsorption

- Model studies – Surface science
  - stainless steel UHV setup with flanges, pumps, pressure gauges, etc.
  - $10^{-10}$  to  $10^{-11}$  mbar base pressure
  - tools and components for preparation, characterization, sample manipulation, resistive heating




manipulator

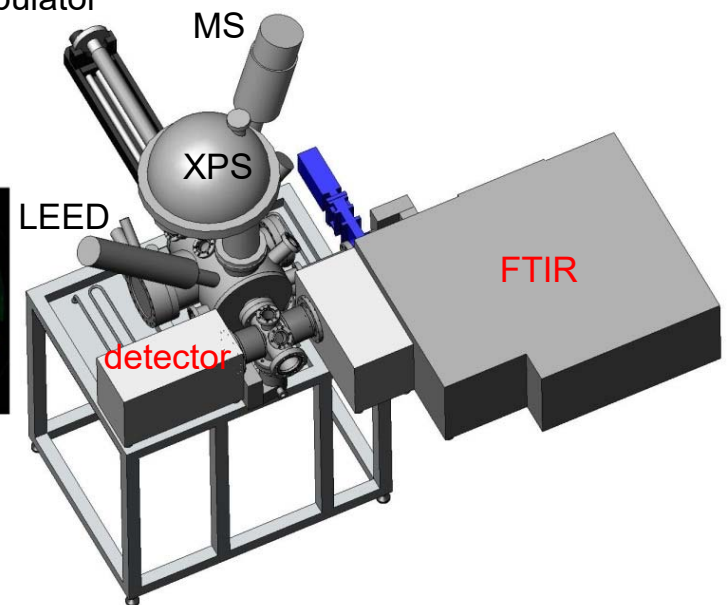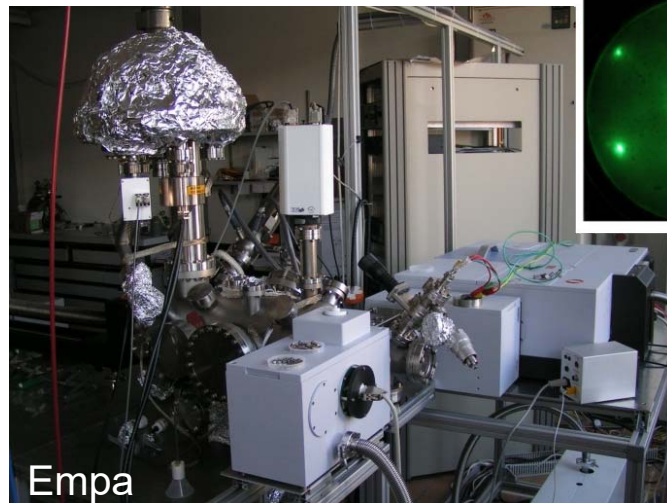




# CO adsorption

- Model studies – Surface science

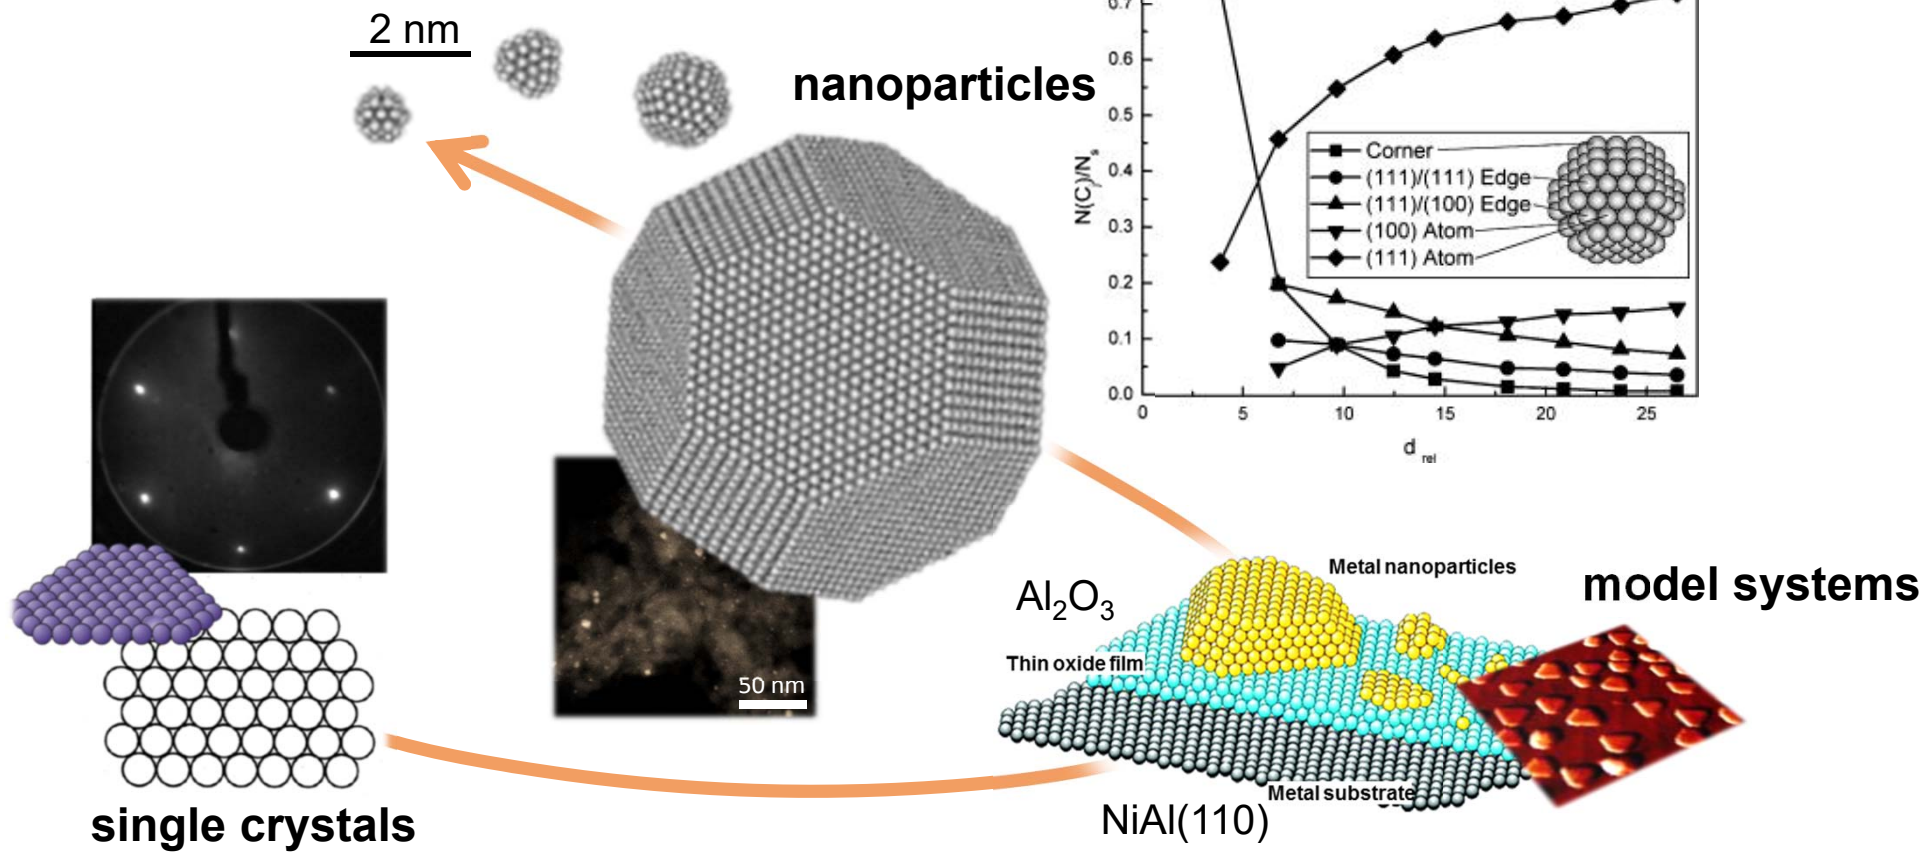


# CO adsorption

- Powders

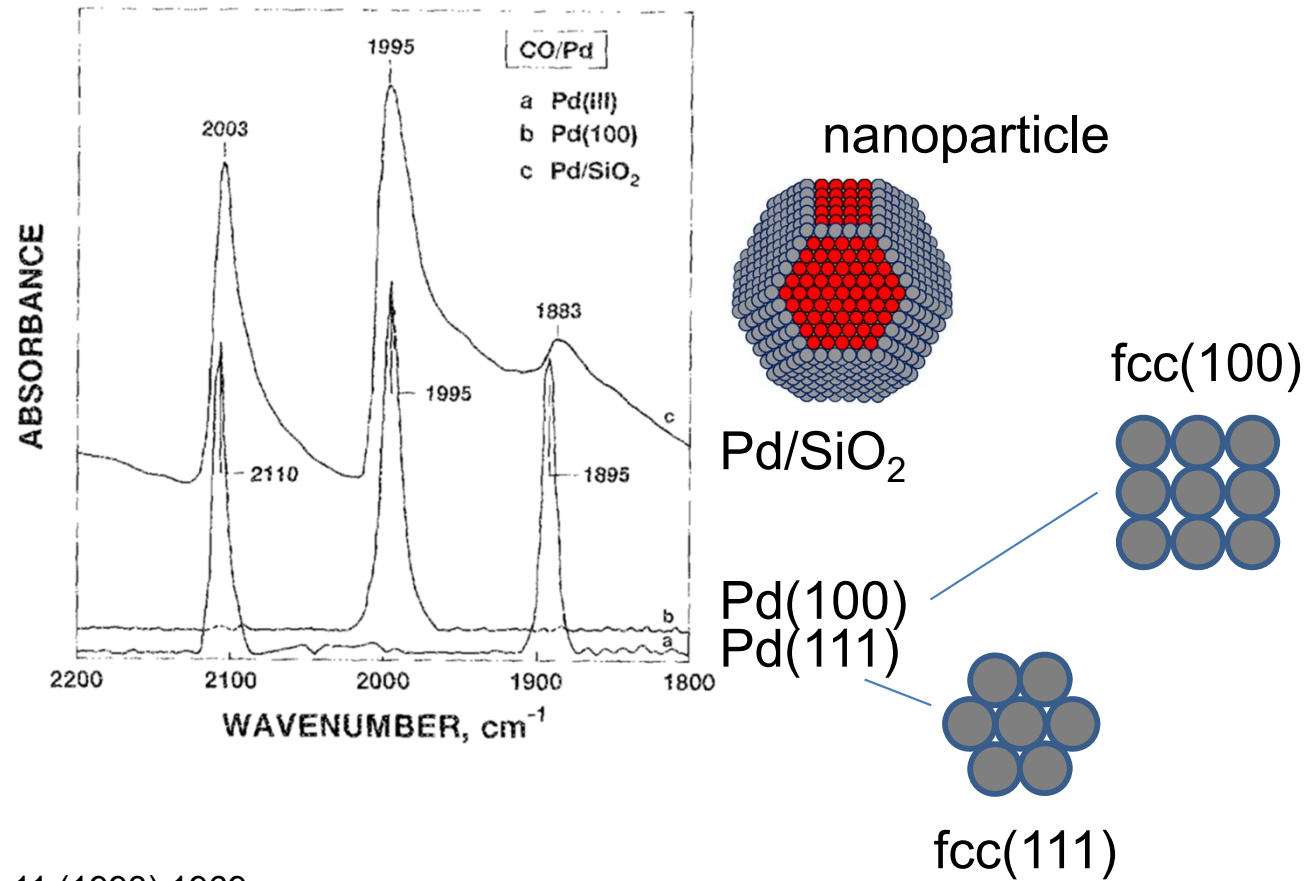

# CO adsorption


- Powders

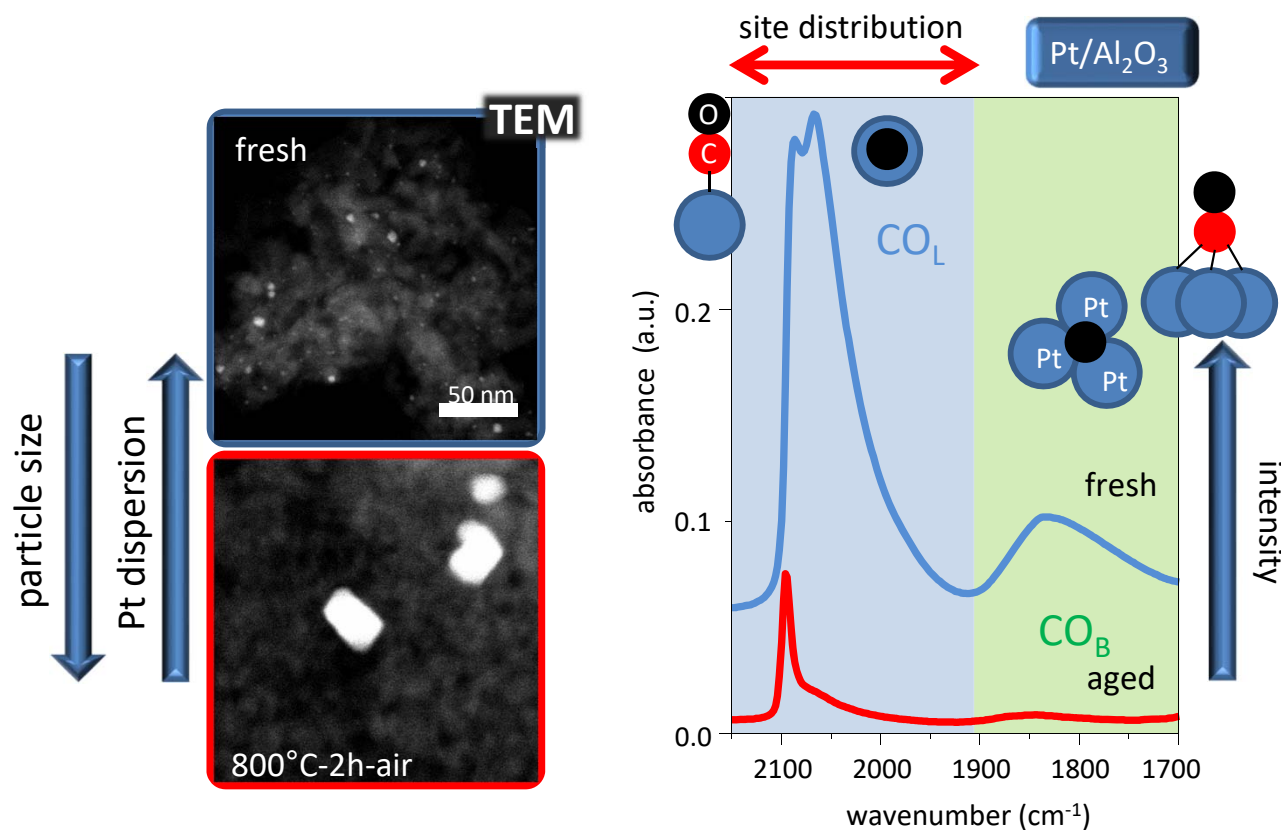



- the larger the particles, the less CO adsorbs (**intensity**)
- the larger the particles, the less the available defects (**nr. of signals**)

# CO adsorption


How does the CO stretching frequency shift when a Pt surface is covered with hydrogen or oxygen?

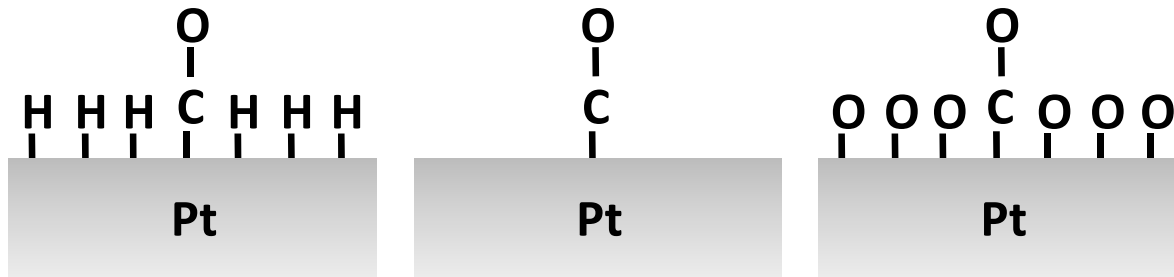


# CO adsorption

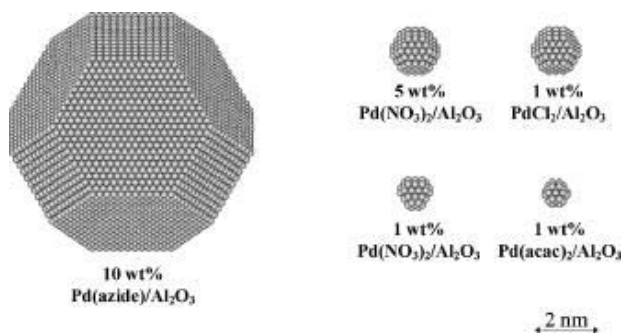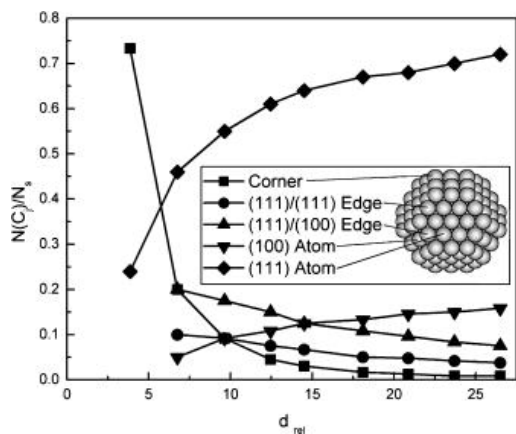


size confirmed by TEM

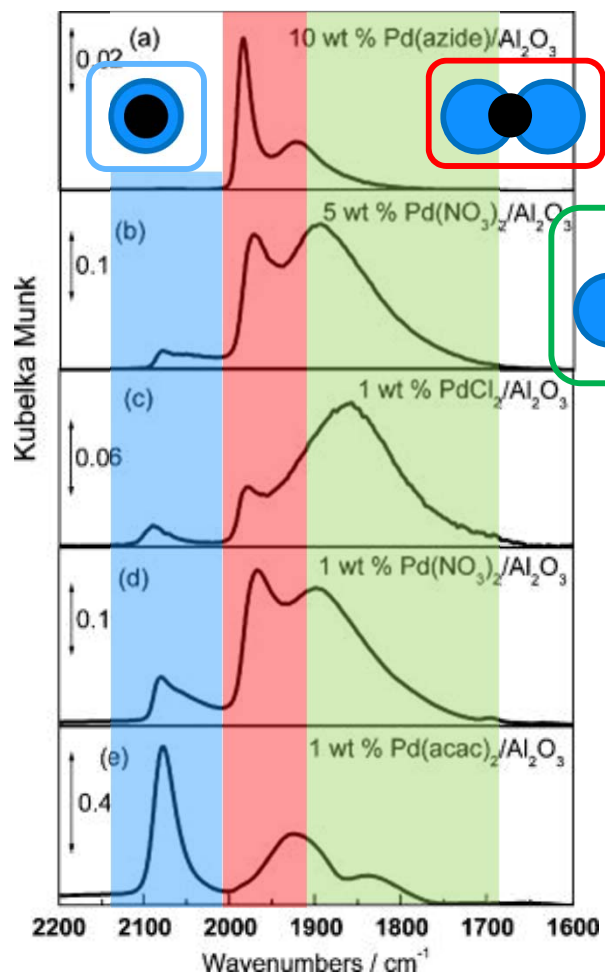

# CO adsorption

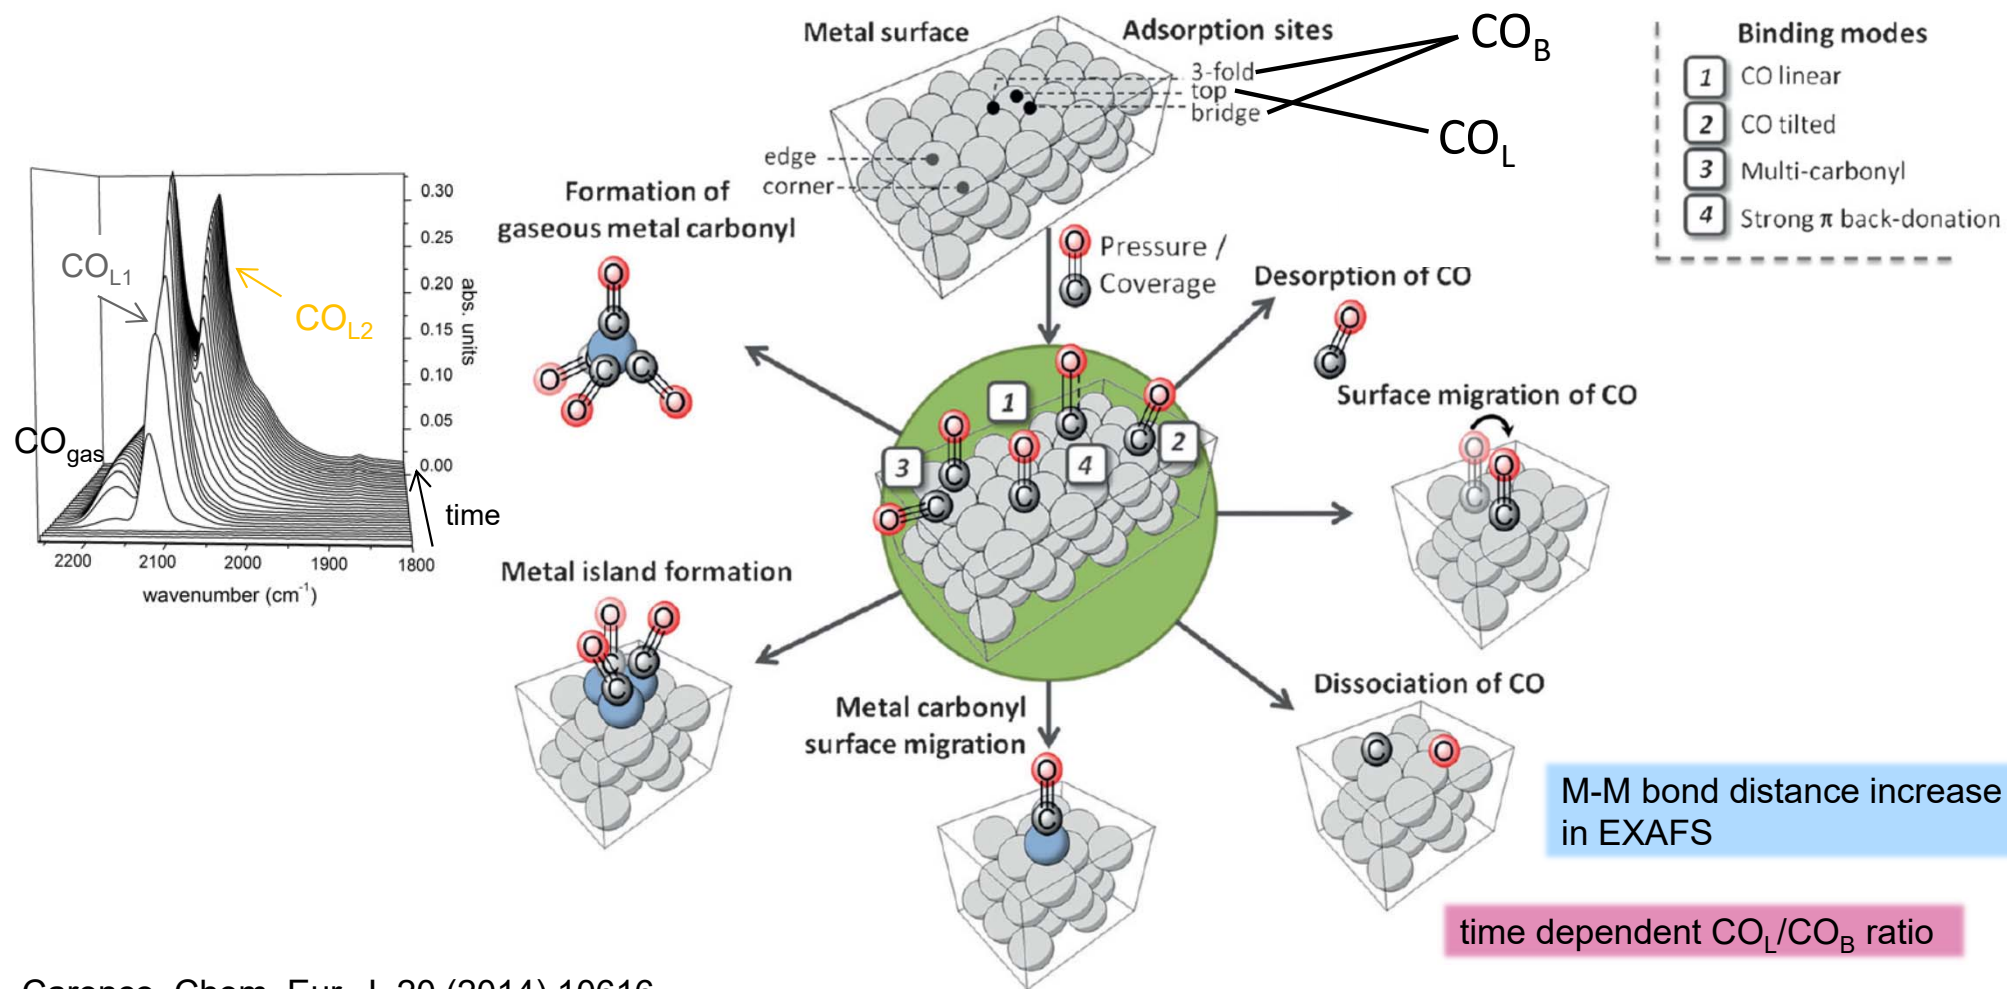

# CO adsorption

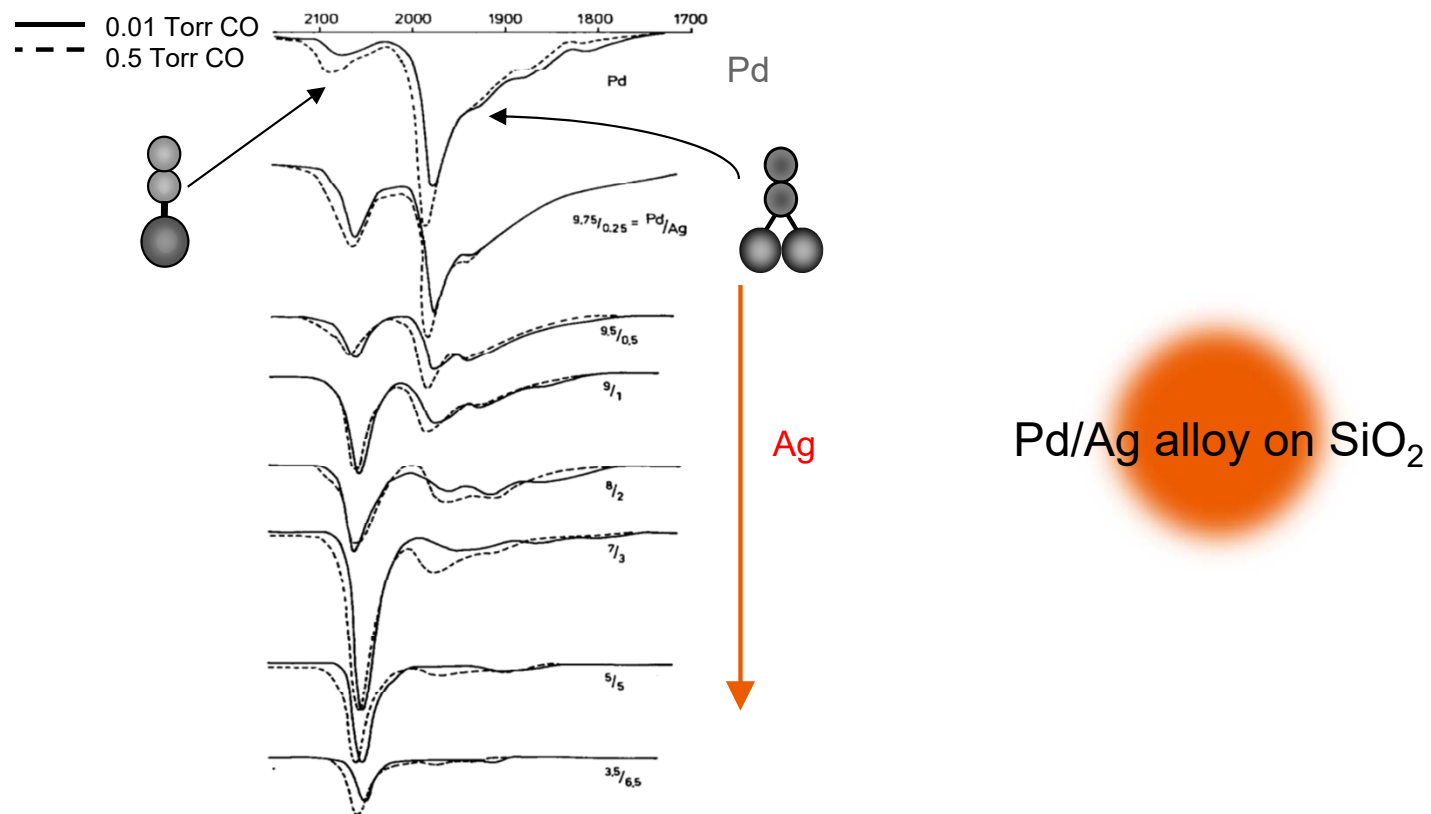

# The surface selection rule


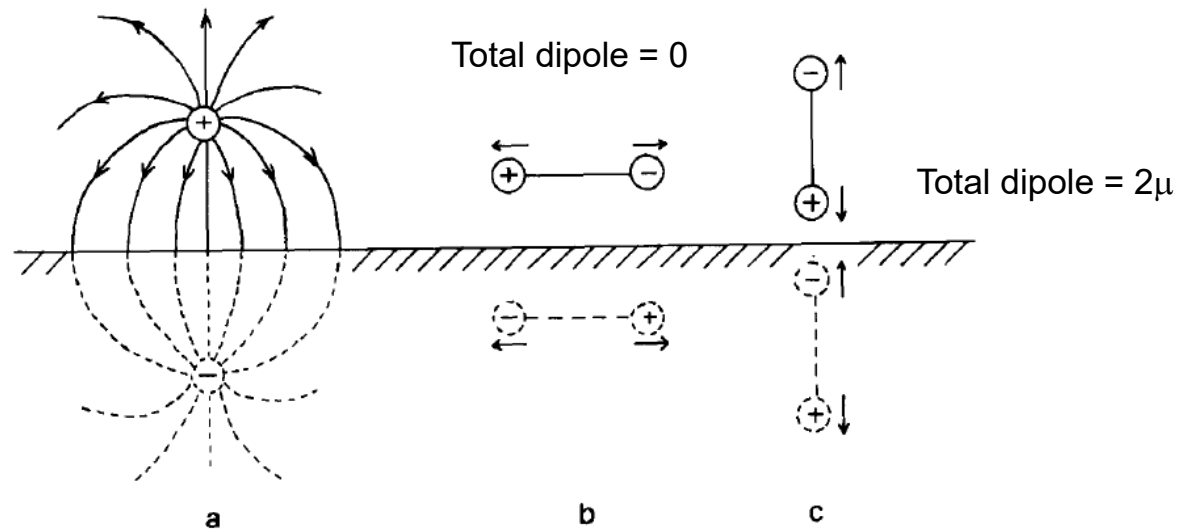


Fig. 1. (a) The lines of force and the electrical "image" resulting from a positive charge over the surface of a conductor (the metal surface is the upper line above the hatched area). (b) The changes during the vibration of a dipole parallel to the surface of the metal; the "image" dipole change is in the opposite direction to the original. (c) The changes during the vibration of a dipole perpendicular to the surface; the "image" dipole change is in the same direction as the original.



# The surface selection rule

- Carboxylate groups


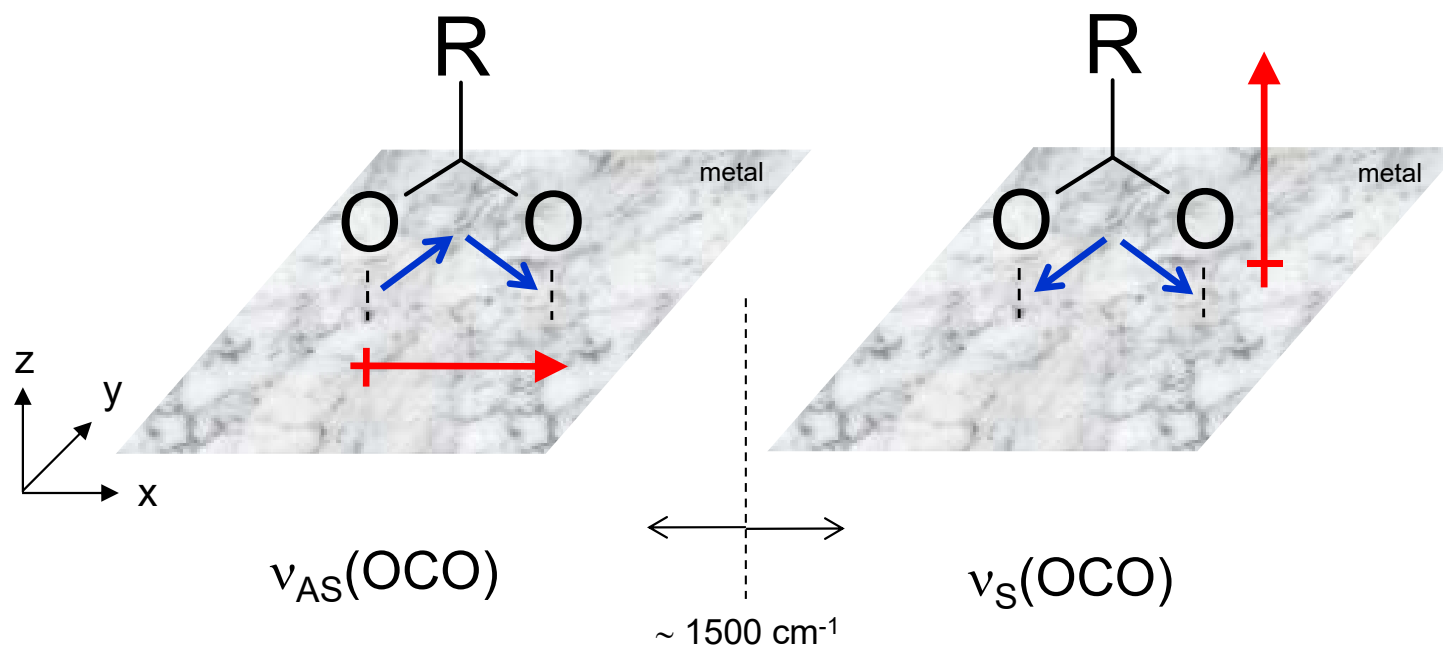


Note that the selection rule can break down for particles smaller than ca. 2 nm


Greenler et al. Surf. Sci. 118 (1982) 415

# Reflection-absorption (IRRAS)


- Also RAIRS; specular/external reflection method

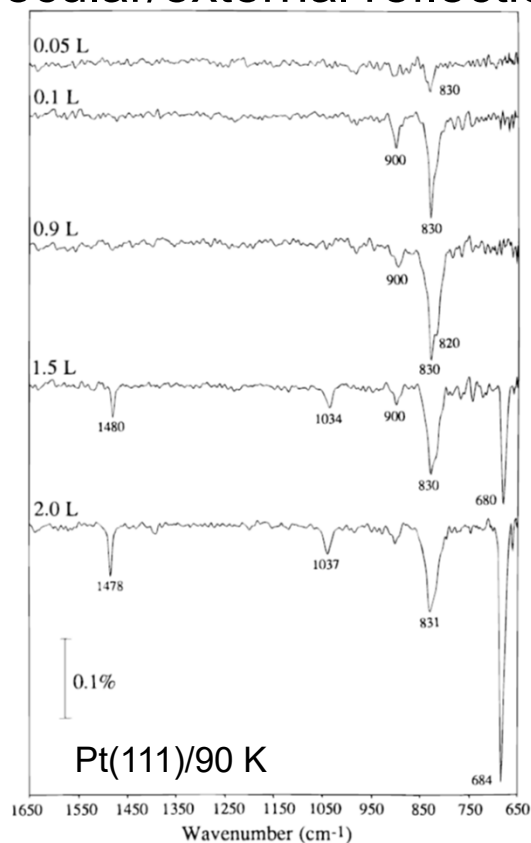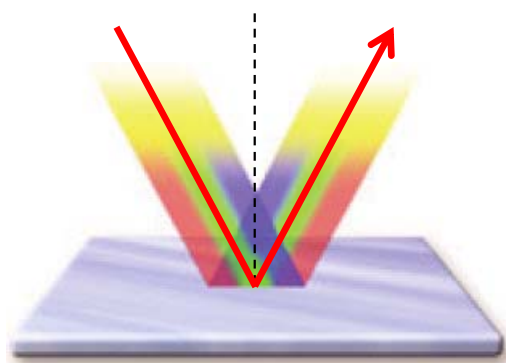

L (Langmuir) = exposure of  $10^{-6}$  Torr gas for 1 s

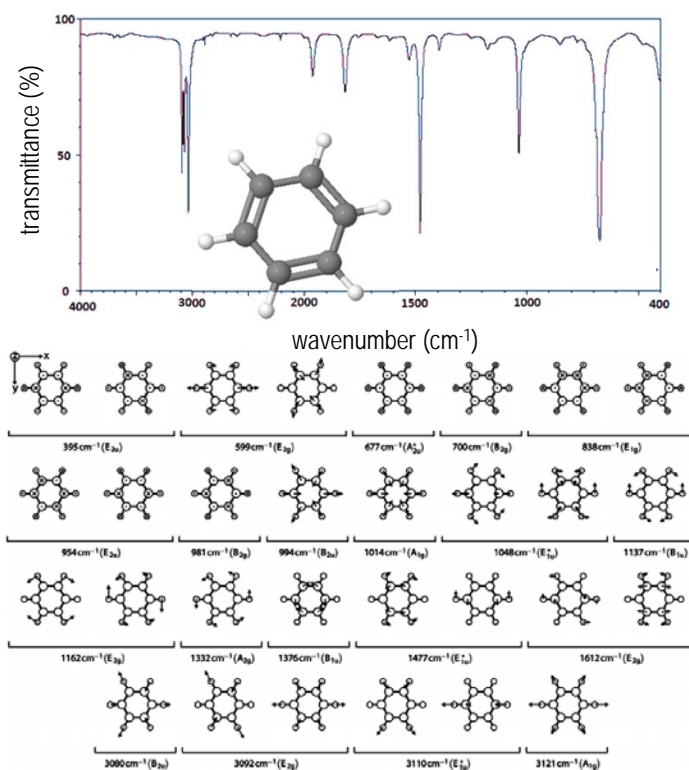


# Reflection-absorption (IRRAS)

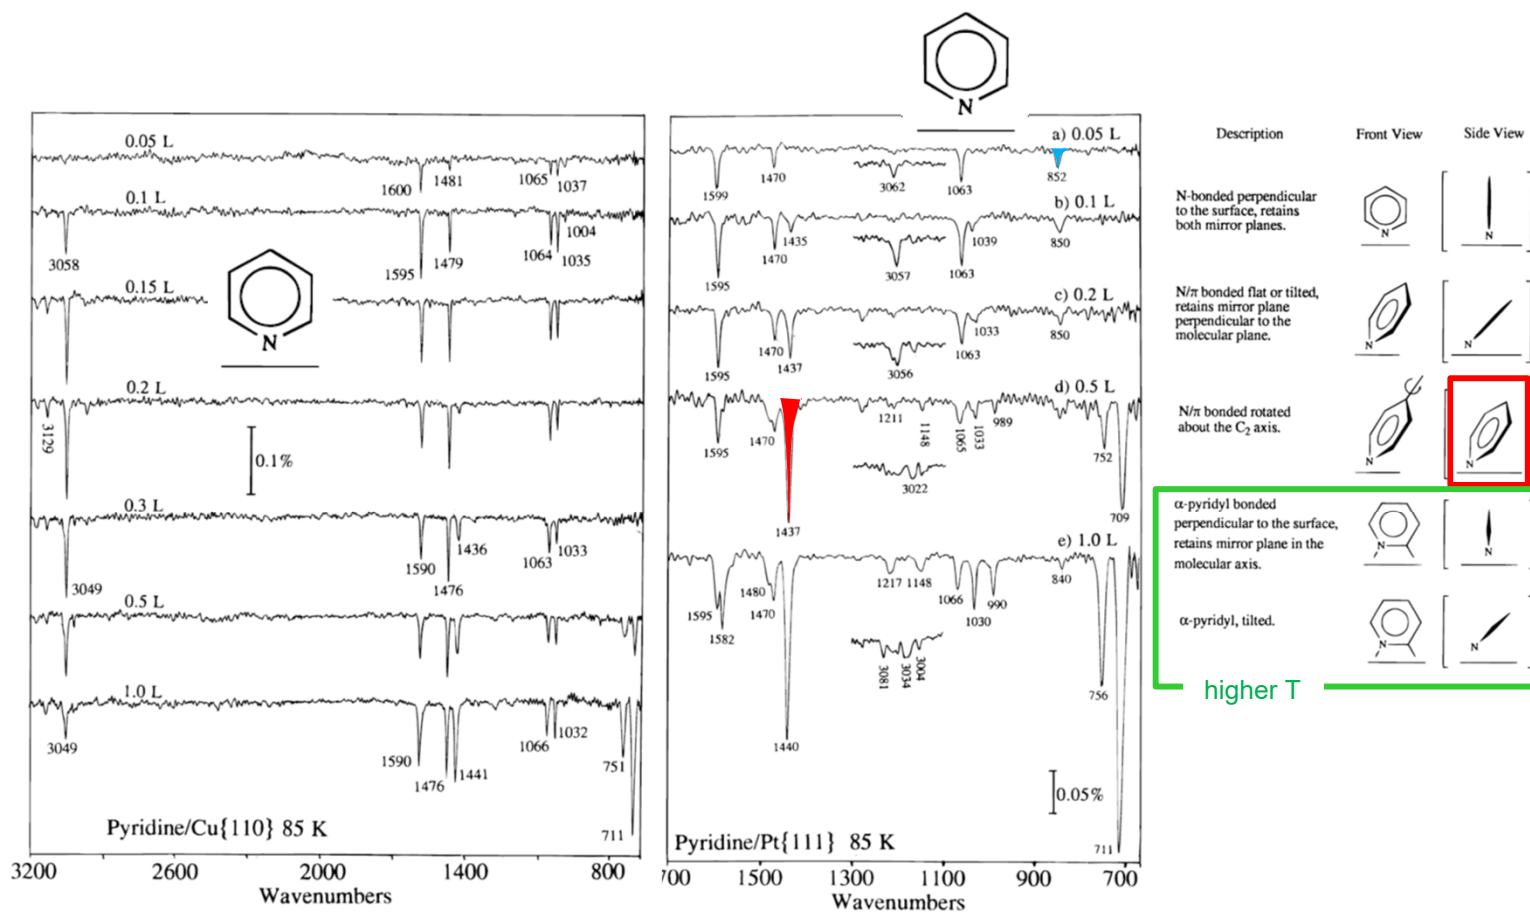

# Reflection-absorption (IRRAS)

- Adsorption of ethylene

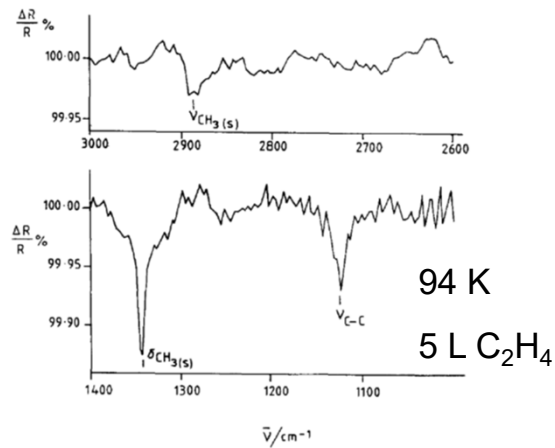


Vibrational assignments of ethyldiyne


Mode	Pt(111) (cm <sup>-1</sup> )		Co <sub>3</sub> (CO) <sub>9</sub> CCH <sub>3</sub> (cm <sup>-1</sup> )
	FT-RAIRS [this work]	EELS [5]	
$\nu_{as}(\text{CH}_3)$	Not allowed	2950 (impact)	2924
$\nu_s(\text{CH}_3)$	2884	2895	2882
$\delta_{as}(\text{CH}_3)$	Not allowed	1420 (impact)	1432
$\delta_s(\text{CH}_3)$	1341	1350	1359
$\nu_{C-C}$	1124	1130	1161
$\rho(\text{CH}_3)$	Not allowed	980 (impact)	1006
$\nu_{C-Pt}$	Below detector cut off	435	~ 600

# Phase-modulation IRRAS (PM-IRRAS)


- Generation of 2 polarizations (photoelastic modulator)
  - excellent gas-phase compensation
  - non-UHV experiments possible
  - highly sensitive, time-resolved studies possible

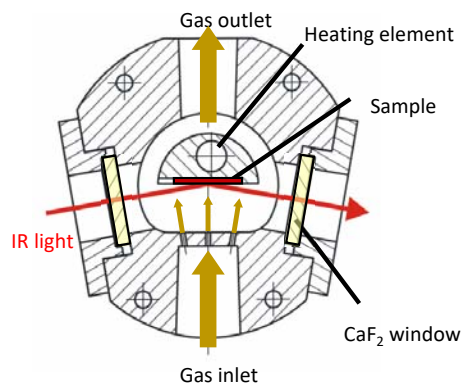


Urakawa et al., *J. Chem. Phys.* 124 (2006) 054717

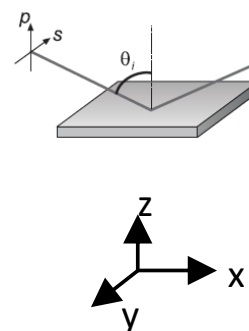

Perpendicular (s-) polarization (y-axis)

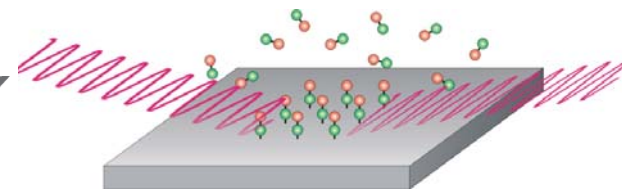

Parallel (p-) polarization (x, z-axis)

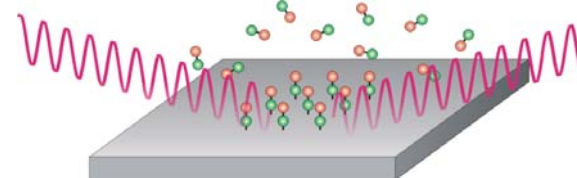

$$R_p - R_s = \Delta R$$

Parallel polarization (surface + gas) - Perpendicular polarization (gas) = Difference (surface)


The surface spectra are often shown in  $\Delta R/R$  ( $R=R_s+R_p$ )

# Acid sites

- Quality and quantity of acid sites | Criteria
  - unequivocal analysis of intermolecular interaction
  - selective interaction with acidic or basic sites
  - sufficient accuracy in frequency shift determination
  - high (and available) extinction coefficients of adsorbed probe
  - appropriate acid (base) strength to induce interaction
  - high specificity (allow discrimination between sites with different strength) - Use different molecules !
  - small molecular size - Use different molecules !
    - pyridine (smaller channels) and picoline (larger channels or surface only)
  - low reactivity under exp. conditions
- Examples
  - acidity of zeolites with different channel sizes
  - acid sites located in all channels


# Probe molecules

- Adsorption of  $\text{NH}_3$

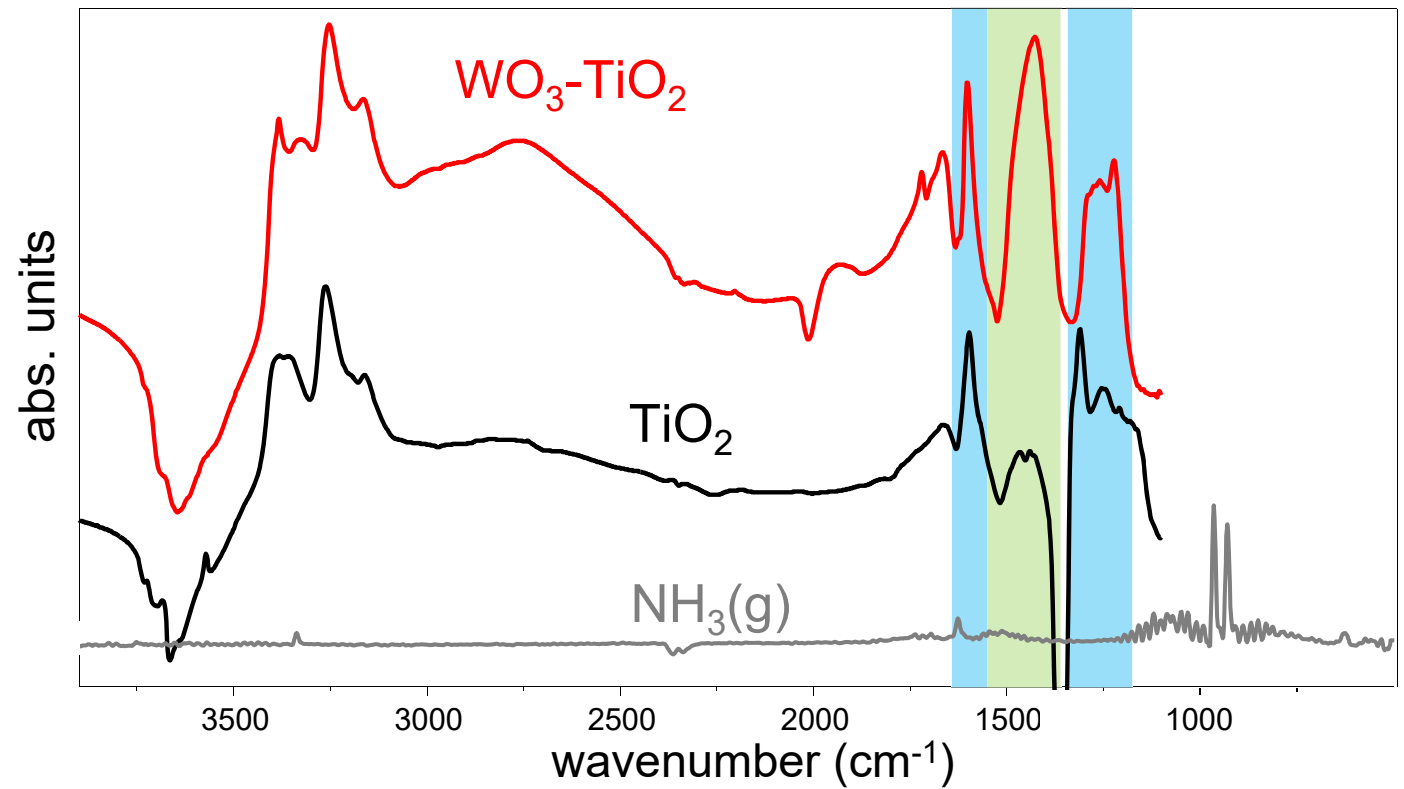

# Probe molecules



- Adsorption of  $\text{NH}_3$

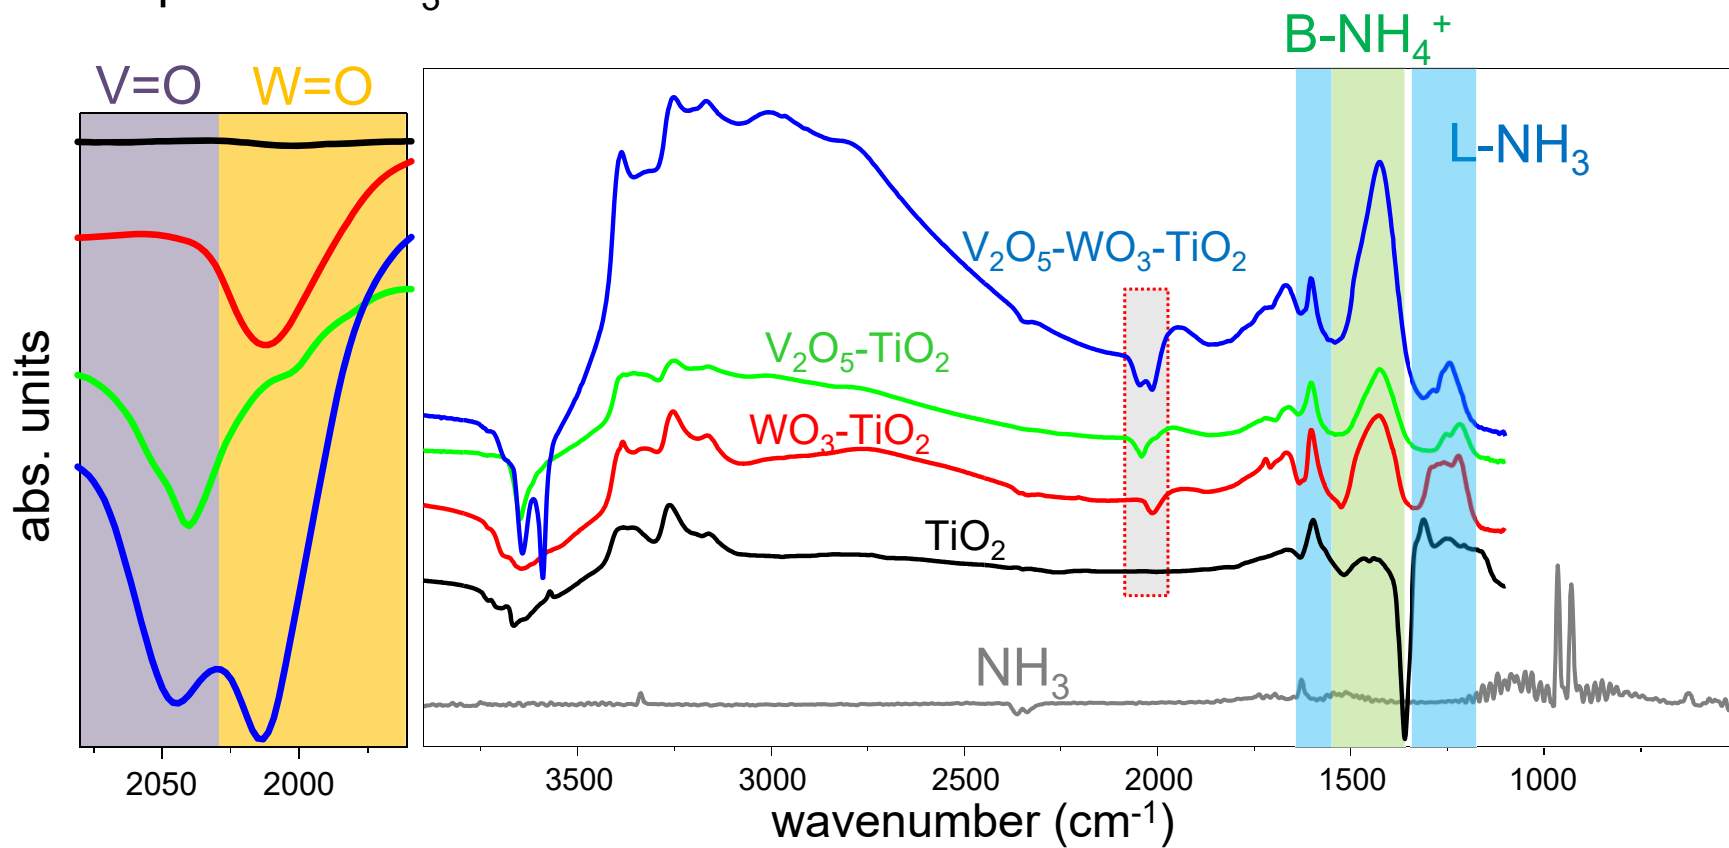




# Acid sites



**BAS**  
Brønsted sites  
(protic)

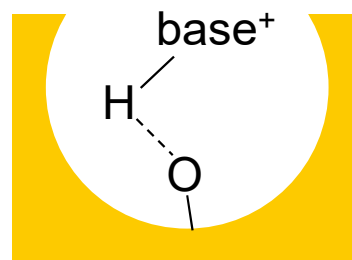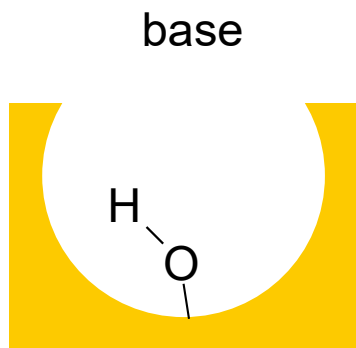

**HB**  
hydrogen bond

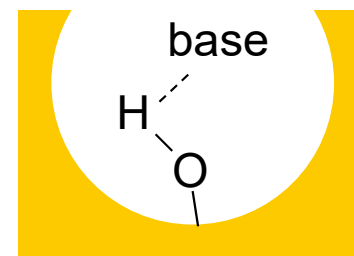


**LAS**  
Lewis sites  
(aprotic)

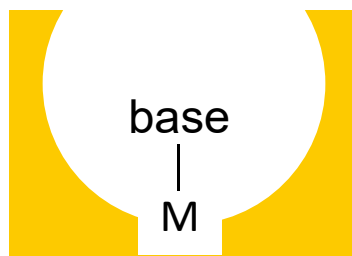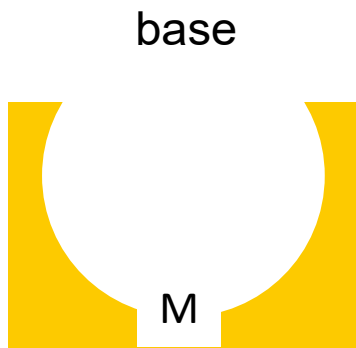


# Acid sites


- Adsorption of  $\text{NH}_3$ 
  - $\text{V}_2\text{O}_5/\text{WO}_3\text{-TiO}_2$

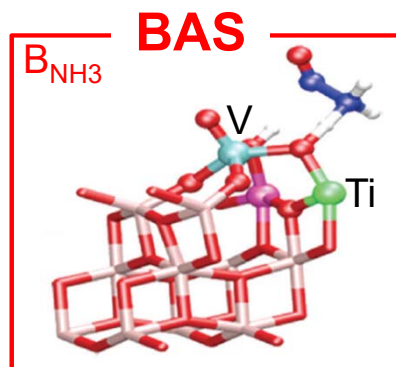

Arnarsson et al., *PCCP* 18 (2016) 17071

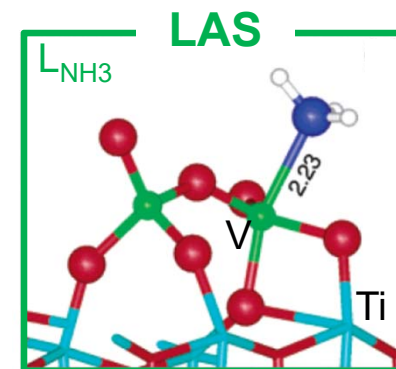


Vittadini et al., *J. Phys. Chem. B Lett.* 109 (2005) 1652

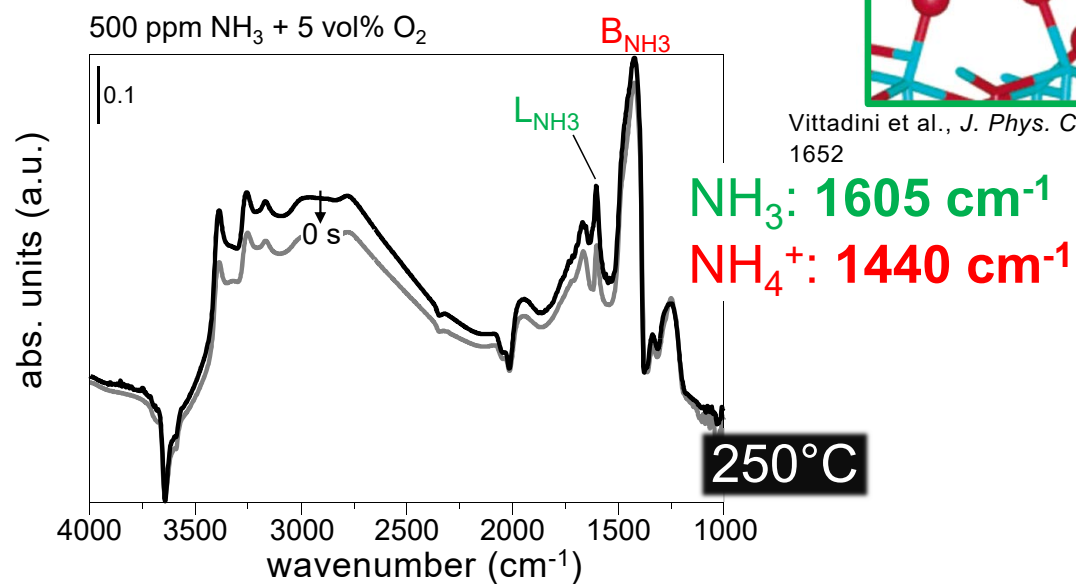

## Acid sites

- Probe molecules for the study of localization of active sites in microporous materials

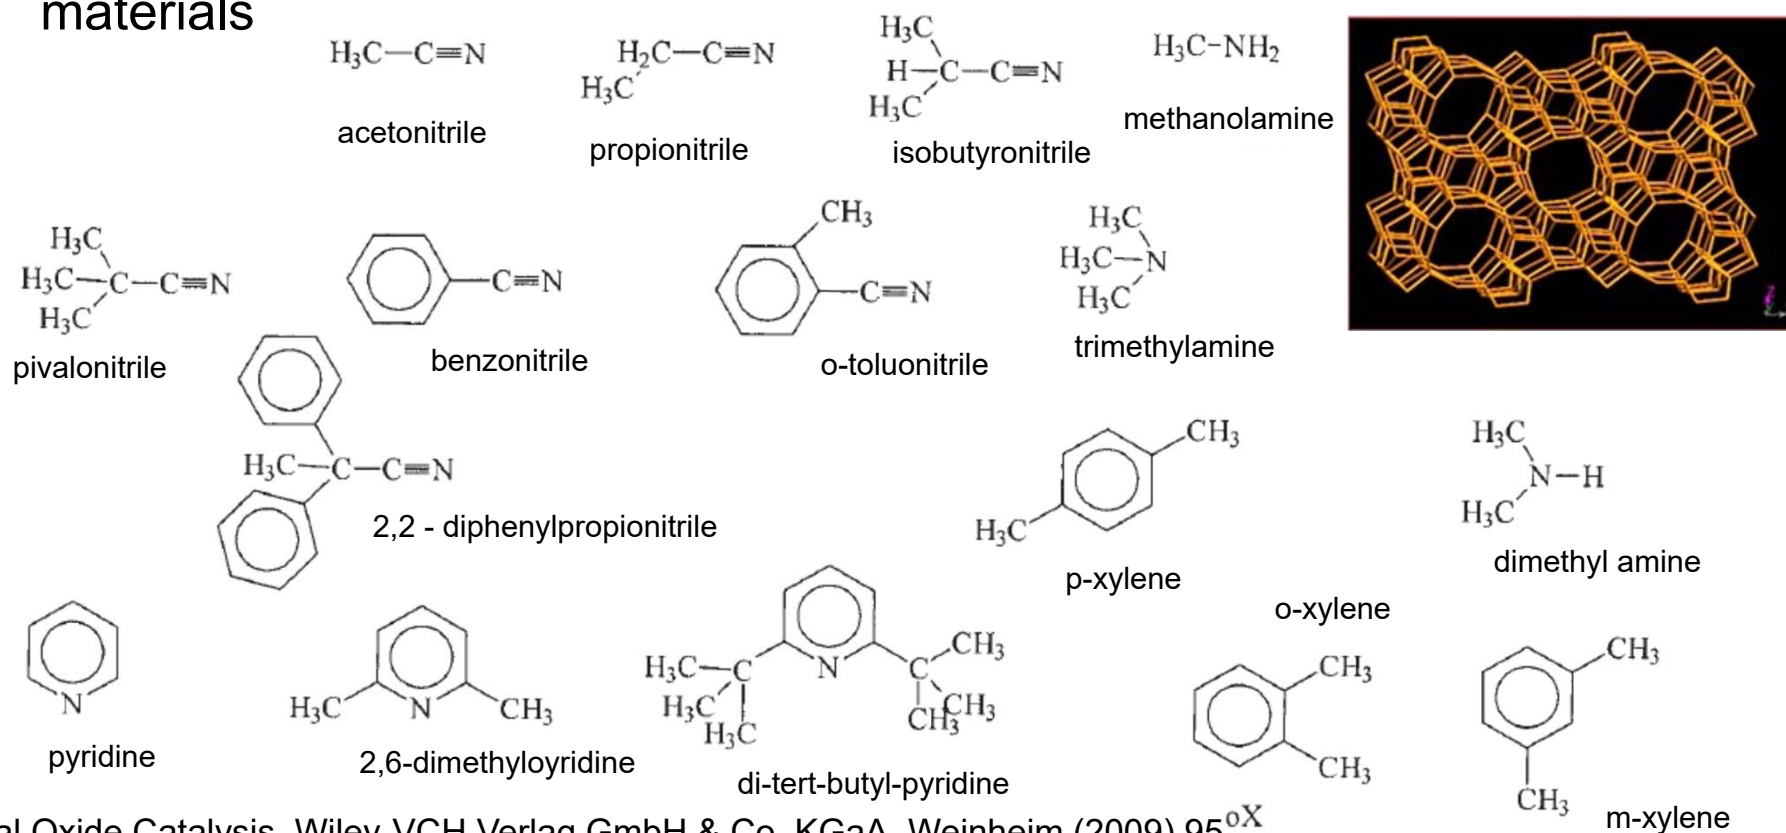

# Acid sites

- Pyridine  
– Transmission

